

TOSHIBA

**DICOM CONFORMANCE STATEMENT
FOR
DIAGNOSTIC ULTRASOUND SYSTEM**

MODEL SSH-880CV *Aplio™ Artida™* V1.50

TOSHIBA MEDICAL SYSTEMS CORPORATION

© TOSHIBA MEDICAL SYSTEMS CORPORATION 2008
ALL RIGHTS RESERVED

Trademarks

“Aplio” and “Artida” are trademarks of Toshiba Medical Systems Corporation.
This document may include trademarks or registered trademarks of other companies.

IMPORTANT!

- (1) No part of this document may be copied or reprinted, in whole or in part, without written permission.
- (2) The contents of this document are subject to change without prior notice and without our legal obligation.

*

1. CONFORMANCE STATEMENT OVERVIEW

Table 1-1 provides an overview of the network services supported by *Aplio™ Artida™*.

**Table 1-1
NETWORK SERVICES**

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Transfer		
Secondary Capture Image Storage	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Ultrasound Multi-frame Image Storage	Yes	Yes
Enhanced SR Storage	Yes	Yes
Storage Commitment		
Storage Commitment Push Model	Yes	No
Workflow Management		
Modality Worklist Information Model – Find	Yes	No
Modality Performed Procedure Step	Yes	No

Table 1-2 provides an overview of the Media Storage Application Profiles supported by *Aplio™ Artida™*.

**Table 1-2
MEDIA SERVICES**

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
Compact Disk – Recordable		
General Purpose CD-R	Yes	Yes
DVD Plus Recordable		
General Purpose DVD	Yes	Yes
USB Media		
General Purpose USB Media	Yes	Yes

*

2. TABLE OF CONTENTS

1.	CONFORMANCE STATEMENT OVERVIEW	i
2.	TABLE OF CONTENTS	a
3.	INTRODUCTION	1
3.1	AUDIENCE	1
3.2	REMARKS	1
3.3	DEFINITIONS, TERMS AND ABBREVIATIONS	2
3.4	REFERENCES	2
4.	NETWORKING	3
4.1	IMPLEMENTATION MODEL	3
4.1.1	Application Data Flow	3
4.1.2	Functional Definition of AEs	5
4.1.3	Sequencing of Real-World Activities	6
4.2	AE SPECIFICATIONS	7
4.2.1	Storage SCU AE Specification	7
4.2.2	Storage Commitment SCU AE Specification	11
4.2.3	MWM SCU AE Specification	16
4.2.4	MPPS SCU AE Specification	21
4.2.5	Storage SCP AE Specification	26
4.3	NETWORK INTERFACES	30
4.3.1	Physical Network Interface	30
4.3.2	Additional Protocols	30
4.4	CONFIGURATION	31
4.4.1	AE Title/Presentation Address Mapping	31
4.4.2	Parameters	31
5.	MEDIA INTERCHANGE	33
5.1	IMPLEMENTATION MODEL	33
5.1.1	Application Data Flow	33
5.1.2	Functional Definition of AEs	33
5.1.3	Sequencing of Real-World Activities	34
5.1.4	File Meta Information for Implementation Class and Version	34
5.2	AE SPECIFICATIONS	35
5.2.1	Offline-Media AE Specification	35
5.3	AUGMENTED AND PRIVATE APPLICATION PROFILES	36
5.3.1	Augmented Application Profiles	36
5.3.2	Private Application Profiles	36
5.4	MEDIA CONFIGURATION	36
6.	SUPPORT OF CHARACTER SETS	37
7.	SECURTIY	38

8.	ANNEXES	39
8.1	IOD CONTENTS	39
8.1.1	Created SOP Instances	39
8.1.2	Usage of Attributes from received IOD's	59
8.1.3	Attribute Mapping	59
8.1.4	Coerced/Modified Fields	59
8.2	DATA DICTIONARY OF PRIVATE ATTRIBUTES	60
8.3	CONTROLLED TERMINOLOGY AND TEMPLATES	60
8.4	GRAYSCALE IMAGE CONSISTENCY	60
8.5	STANDARD EXTENDED/SPECIALIZED/PRIVATE SOP CLASSES	60
8.6	PRIVATE TRANSFER SYNTAXES	60

3. INTRODUCTION

3.1 AUDIENCE

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

3.2 REMARKS

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Toshiba Medical Systems and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Toshiba Medical Systems and non-Toshiba Medical Systems equipment.
- Test procedures should be defined to validate the desired level of connectivity.
- The DICOM standard will evolve to meet the users' future requirements. Toshiba Medical Systems is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.

3.3 DEFINITIONS, TERMS AND ABBREVIATIONS

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Abbreviations and terms are as follows:

AE	Application Entity
ASCE	Association Control Service Element
CD-R	Compact Disk Recordable
DIMSE	DICOM Message Service Element
DVD	A trademark of the DVD forum that is not an abbreviation
DVD+R	DVD Plus Recordable
FSC	File-Set Creator
FSR	File-Set Reader
FSU	File-Set Updater
IE	Information Entity
IOD	Information Object Definition
ISO	International Standard Organization
MPPS	Modality Performed Procedure Step
MSPS	Modality Scheduled Procedure Step
MWM	Modality Worklist Management
PDU	Protocol Data Unit
SCU	Service Class User (DICOM client)
SCP	Service Class Provider (DICOM server)
SOP	Service-Object Pair
UID	Unique Identifier
USB	Universal Serial Bus


3.4 REFERENCES

[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-3.18, 2008

4. NETWORKING

4.1 IMPLEMENTATION MODEL

4.1.1 Application Data Flow

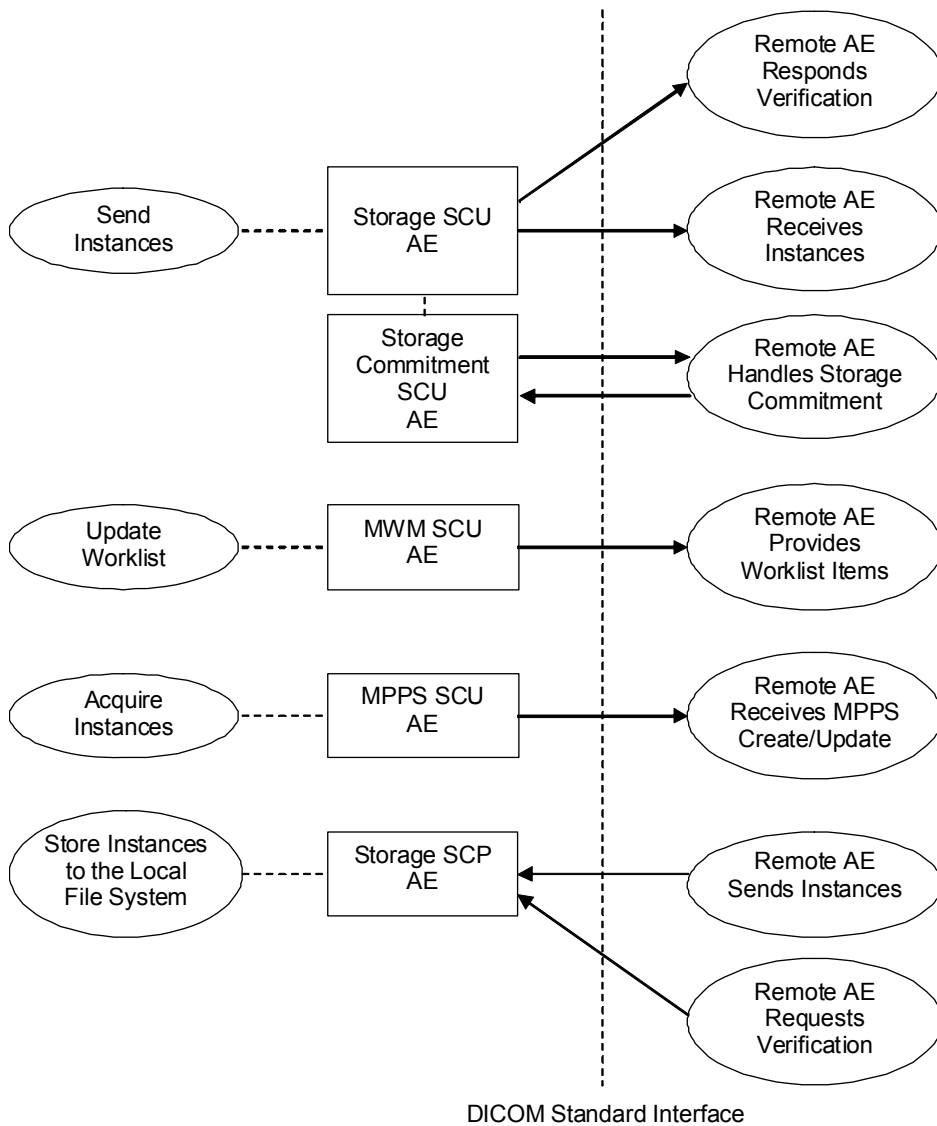

**Figure 4.1-1
APPLICATION DATA FLOW DIAGRAM**

- The Storage SCU AE sends instances to a remote AE. It is associated with the local real-world activity “Send Instances”. “Send Instances” is performed upon user request for specific instances selected. If the remote AE is configured as a Storage Commitment SCP AE, the Storage SCU AE will send a storage commitment request to the Storage Commitment SCU AE. The Storage SCU AE can also issue C-ECHO requests as a Verification SCU.
- Receiving the storage commitment request from the Storage SCU AE, the Storage Commitment SCU AE will request Storage Commitment and if a commitment is successfully obtained will record this information in the local database.
- The MWM SCU AE receives worklist information from a remote AE. It is associated with the local real-world activity “Update Worklist”. When the “Update Worklist” is performed the MWM SCU AE queries a remote AE for worklist items and provides the set of worklist items matching the query request. “Update Worklist” is performed manually or automatically.
- The MPPS SCU AE sends MPPS information to a remote AE. It is associated with the local real-world activity “Acquire Instances”. When the “Acquire Instances” is performed the MPPS SCU AE creates and updates Modality Performed Procedure Step instances managed by a remote AE. Acquisition of instances will result in automated creation of an MPPS instance. Completion of the MPPS is performed as the result of an operator action.
- The Storage SCP AE receives incoming instances. It is associated with the local real-world activity “Store Instances to the Local File System”. “Store Instances to the Local File System” stores the received instances to the local file system. The Storage SCP AE can also respond to C-ECHO requests as a Verification SCP.

4.1.2 Functional Definition of AEs

4.1.2.1 Functional Definition of Storage SCU AE

The existence of a send-job queue entry with associated network destination will activate the Storage SCU AE. An association request is sent to the destination AE and upon successful negotiation of a Presentation Context the instance transfer is started. If the instance transfer fails, the Storage SCU AE will retry this send-job automatically. If the remote AE is configured as a Storage Commitment SCP AE, the Storage SCU AE will send a storage commitment request to the Storage Commitment SCU AE. The Storage SCU AE can also issue C-ECHO requests as a Verification SCU for service purposes when a remote AE is configured.

4.1.2.2 Functional Definition of Storage Commitment SCU AE

Receiving the storage commitment request from the Storage SCU AE, the Storage Commitment SCU AE will request Storage Commitment and if a commitment is successfully obtained will record this information in the local database.

4.1.2.3 Functional Definition of MWM SCU AE

The MWM SCU AE attempts to download a worklist from a remote node. If the MWM SCU AE establishes an association to a remote AE, it will transfer patient's information and worklist items via the open association. The results will be displayed in a separate list. The patient's information will be used for the patient registration.


4.1.2.4 Functional Definition of MPPS SCU AE

The MPPS SCU AE performs the creation of an MPPS Instance automatically when the user selects and starts a worklist item. Further updates on the MPPS data can be performed when the user completes the acquisition.

4.1.2.5 Functional Definition of Storage SCP AE

The Storage SCP AE waits for another application to connect at the presentation address configured for its Application Entity Title. The Storage SCP AE will accept Associations with Presentation Contexts for SOP Classes of the Verification and Storage Service Classes. Any instances received on such Presentation Contexts will be stored to the local file system.

4.1.3 Sequencing of Real-World Activities

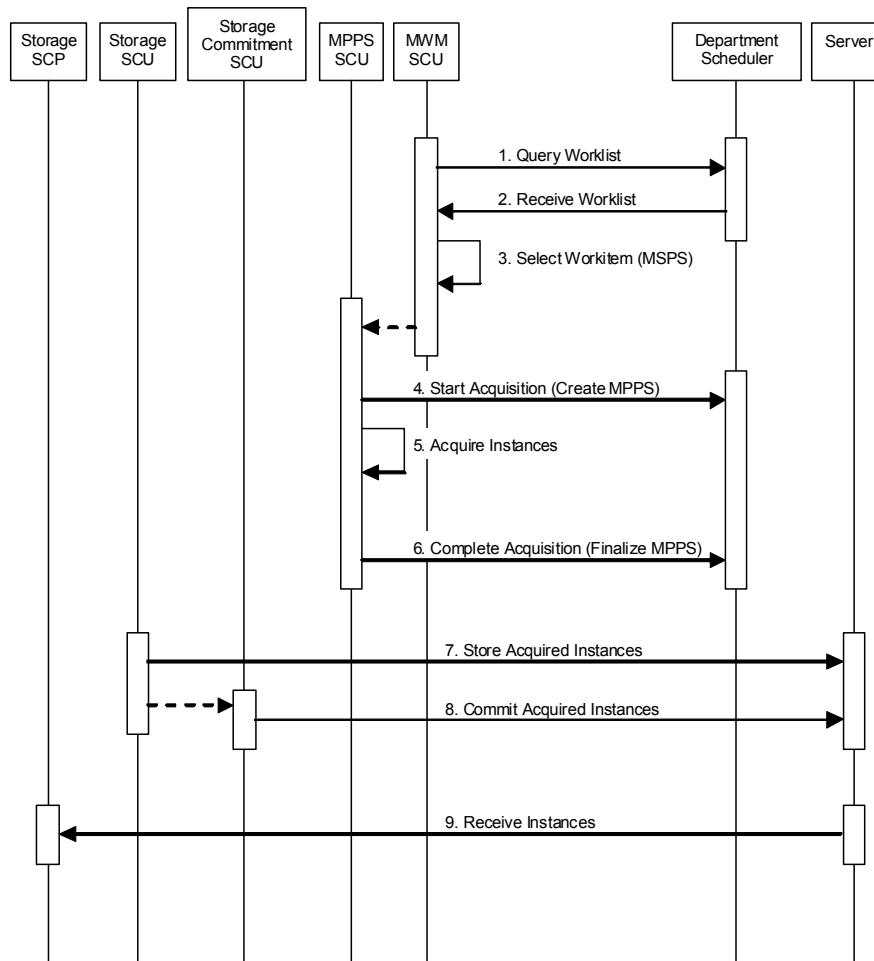

**Figure 4.1-2
SEQUENCING CONSTRAINTS**

Under typical scheduled workflow conditions the sequencing constraints illustrated in Figure 4.1-2 apply:

1. Query Worklist
2. Receive Worklist of Modality Scheduled Procedure Steps (MSPS)
3. Select Workitem (MSPS) from Worklist
4. Start Acquisition and Create MPPS
5. Acquire Instances
6. Complete Acquisition and Finalize MPPS
7. Store Acquired Instances
8. Commit Acquired Instances
9. Receive Instances

Other workflow situations (e.g. unscheduled procedure steps) will have other sequencing constraints. Some activities may be omitted according to situations.

4.2 AE SPECIFICATIONS

4.2.1 Storage SCU AE Specification

4.2.1.1 SOP Classes

The Storage SCU AE provides Standard Conformance to the following SOP Classes:

Table 4.2-1
SOP CLASSES FOR THE STORAGE SCU AE

SOP Class Name	SOP Class UID	SCU	SCP
Verification	1.2.840.10008.1.1	Yes	No
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7		
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1		
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1		
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22		

4.2.1.2 Association Policies

4.2.1.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

Table 4.2-2
DICOM APPLICATION CONTEXT FOR THE STORAGE SCU AE

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

4.2.1.2.2 Number of Associations

The Storage SCU AE can initiate up to three associations at a time for each destination to which a transfer request is being processed in the active job queue list. Up to ten jobs, that instances will be sent to the different remote hosts, will be active at a time, the other remains pending until the active job is completed or failed.

Table 4.2-3
NUMBER OF ASSOCIATIONS INITIATED FOR THE STORAGE SCU AE

Maximum number of simultaneous associations	10
---	----

4.2.1.2.3 Asynchronous Nature

The Storage SCU AE does not support asynchronous communication (multiple outstanding transactions over a single association).

Table 4.2-4
ASYNCHRONOUS NATURE FOR THE STORAGE SCU AE

Maximum number of outstanding asynchronous transactions	1
---	---

4.2.1.2.4 Implementation Identifying Information

The implementation information for the Storage SCU AE is:

Table 4.2-5
DICOM IMPLEMENTATION CLASS AND VERSION FOR THE STORAGE SCU AE

Implementation Class UID	1.2.392.200036.9116.6.15.1000.1
Implementation Version Name	TM_ARTIDA_1.0

4.2.1.3 Association Initiation Policy

4.2.1.3.1 Activity – Send Instances

4.2.1.3.1.1 Description and Sequencing of Activities

The Storage SCU AE attempts to initiate a new association in order to issue a storage request (C-STORE). If the job contains multiple instances then multiple C-STORE requests will be issued over the same association. If the instance transfer fails, the Storage SCU AE will retry this send-job automatically.

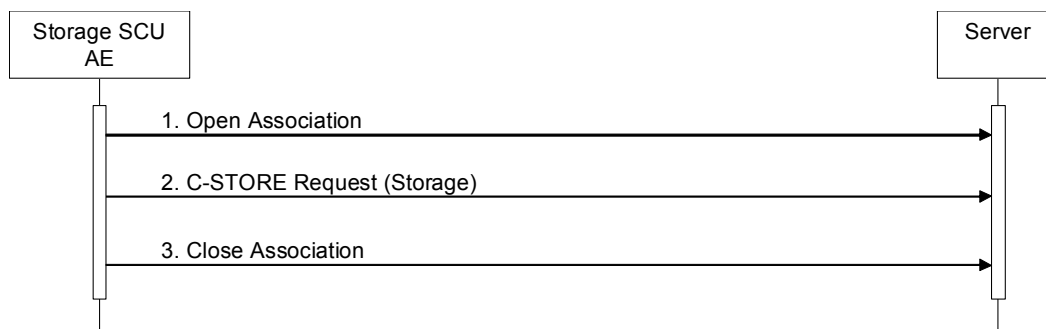


Figure 4.2-1
SEQUENCING OF ACTIVITY – SEND INSTANCES

A possible sequence of interactions between the Storage SCU AE and a Server (e.g. a storage or archive device supporting the Storage SOP Classes as an SCP) is illustrated in the Figure above:

1. The Storage SCU AE opens an association with the Server.
2. Acquired instances are transmitted to the Server using a storage request (C-STORE) and the Server replies with a C-STORE response (status success).
3. The Storage SCU AE closes the association with the Server.

4.2.1.3.1.2 Proposed Presentation Contexts

The Storage SCU AE will propose the Presentation Contexts in the following table that shows a Presentation Context Item a row:

**Table 4.2-6
PROPOSED PRESENTATION CONTEXTS FOR ACTIVITY SEND INSTANCES**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCU	None
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	RLE Lossless	1.2.840.10008.1.2.5	SCU	None
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCU	None
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	RLE Lossless	1.2.840.10008.1.2.5	SCU	None
US Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None
US Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
US Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCU	None
US Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	RLE Lossless	1.2.840.10008.1.2.5	SCU	None
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Implicit VR Little Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1	SCU	None

4.2.1.3.1.3 SOP Specific Conformance for Storage SOP Classes

The Storage SCU AE provides standard conformance to the Storage Service Class as an SCU.

The behavior of Storage SCU AE when encountering status codes in a C-STORE response is summarized in the table below:

**Table 4.2-7
STORAGE C-STORE RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Status Code	Behavior
Success	Success	0000	The SCP has successfully stored the SOP Instance. If all SOP Instances in a send job have status success then the job is marked as complete.
*	*	Any other status code	The association is aborted and the send job is marked as failed. The status meaning is logged and the job failure is reported to the user via the job control application.

The behavior of Storage SCU AE during communication failure is summarized in the table below:

**Table 4.2-8
STORAGE COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	The association is aborted and the send job is marked as failed. The reason is logged and the job failure is reported to the user via the job control application.
Association aborted by the SCP or network layers	The send job is marked as failed. The reason is logged and the job failure is reported to the user via the job control application.

If the instance transfer fails, the Storage SCU AE will retry this send-job automatically. The number of retries is configurable.

The contents of Storage SOP Instances created by the Storage SCU AE conform to the IOD definitions and are described in section 8.1.

4.2.2 Storage Commitment SCU AE Specification

4.2.2.1 SOP Classes

The Storage Commitment SCU AE provides Standard Conformance to the following SOP Classes:

Table 4.2-9
SOP CLASSES FOR THE STORAGE COMMITMENT SCU AE

SOP Class Name	SOP Class UID	SCU	SCP
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No

4.2.2.2 Association Policies

4.2.2.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

Table 4.2-10
DICOM APPLICATION CONTEXT FOR THE STORAGE COMMITMENT SCU AE

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

4.2.2.2.2 Number of Associations

The Storage Commitment SCU AE can initiate up to ten associations at a time.

Table 4.2-11
NUMBER OF ASSOCIATIONS INITIATED FOR THE STORAGE COMMITMENT SCU AE

Maximum number of simultaneous associations	10
---	----

The Storage Commitment SCU AE accepts associations to receive N-EVENT-REPORT notifications for the Storage Commitment Push Model SOP Class.

Table 4.2-12
NUMBER OF ASSOCIATIONS ACCEPTED FOR THE STORAGE COMMITMENT SCU AE

Maximum number of simultaneous associations	10
---	----

4.2.2.2.3 Asynchronous Nature

The Storage Commitment SCU AE does not support asynchronous communication (multiple outstanding transactions over a single association).

Table 4.2-13
ASYNCHRONOUS NATURE FOR THE STORAGE COMMITMENT SCU AE

Maximum number of outstanding asynchronous transactions	1
---	---

4.2.2.2.4 Implementation Identifying Information

The implementation information for the Storage Commitment SCU AE is:

Table 4.2-14
DICOM IMPLEMENTATION CLASS AND VERSION FOR THE STORAGE COMMITMENT SCU AE

Implementation Class UID	1.2.392.200036.9116.6.15.1000.1
Implementation Version Name	TM_ARTIDA_1.0

4.2.2.3 Association Initiation Policy

4.2.2.3.1 Activity – Commit Sent Instances

4.2.2.3.1.1 Description and Sequencing of Activities

If the remote AE is configured as a Storage Commitment SCP AE, the Storage Commitment SCU AE will, after all instances have been sent, transmit a single storage commitment request (N-ACTION). Upon receiving the N-ACTION response the Storage Commitment SCU AE will release the association. The notification of storage commitment (N-EVENT-REPORT) will be received over a separate association.

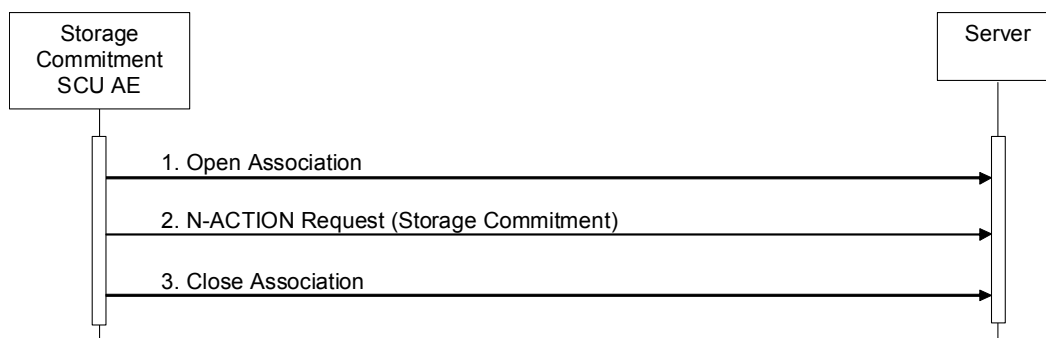


Figure 4.2-2
SEQUENCING OF ACTIVITY – COMMIT SENT INSTANCES

A possible sequence of interactions between the Storage Commitment SCU AE and a Server (e.g. a storage or archive device supporting the Storage Commitment SOP Classes as an SCP) is illustrated in the Figure above:

1. The Storage Commitment SCU AE opens an association with the Server.
2. A storage commitment request (N-ACTION) is transmitted to the Server to obtain storage commitment of previously transmitted instances. The Server replies with an N-ACTION response indicating the request has been received and is being processed.
3. The Storage Commitment SCU AE closes the association with the Server.

Note: The N-EVENT-REPORT will be sent over a separate association initiated by the Server.
(see Section 4.2.2.4.1)

4.2.2.3.1.2 Proposed Presentation Contexts

The Storage Commitment SCU AE will propose the Presentation Contexts shown in the following table:

**Table 4.2-15
PROPOSED PRESENTATION CONTEXTS FOR ACTIVITY COMMIT SENT INSTANCES**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

A Presentation Context for the Storage Commitment Push Model will only be proposed if the remote AE is configured as a Storage Commitment SCP AE.

4.2.2.3.1.3 SOP Specific Conformance for Storage Commitment SOP Class

4.2.2.3.1.3.1 Storage Commitment Operations (N-ACTION)

The Storage Commitment SCU AE provides standard conformance to the Storage Commitment Service Class as an SCU.

The Storage Commitment SCU AE will request storage commitment for instances of the Storage SOP Classes if the remote AE is configured as a Storage Commitment SCP AE and a presentation context for the Storage Commitment Push Model has been accepted.

The behavior of Storage SCU Commitment AE when encountering status codes in an N-ACTION response is summarized in the table below:

**Table 4.2-16
STORAGE COMMITMENT N-ACTION RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Status Code	Behavior
Success	Success	0000	The request for storage commitment is considered successfully sent. A timer is started which will expire if no N-EVENT-REPORT for the Transaction UID is received within a configurable timeout period.
*	*	Any other status code	The association is aborted and the request for storage commitment is marked as failed.

The behavior of Storage Commitment AE during communication failure is summarized in the table below:

**Table 4.2-17
STORAGE COMMITMENT COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	The association is aborted and the send job is marked as failed. The reason is logged and the job failure is reported to the user via the job control application.
Association aborted by the SCP or network layers	The send job is marked as failed. The reason is logged and the job failure is reported to the user via the job control application.

4.2.2.4 Association Acceptance Policy

4.2.2.4.1 Activity – Receive Storage Commitment Response

4.2.2.4.1.1 Description and Sequencing of Activities

The Storage Commitment SCU AE will accept associations in order to receive responses to a storage commitment request.

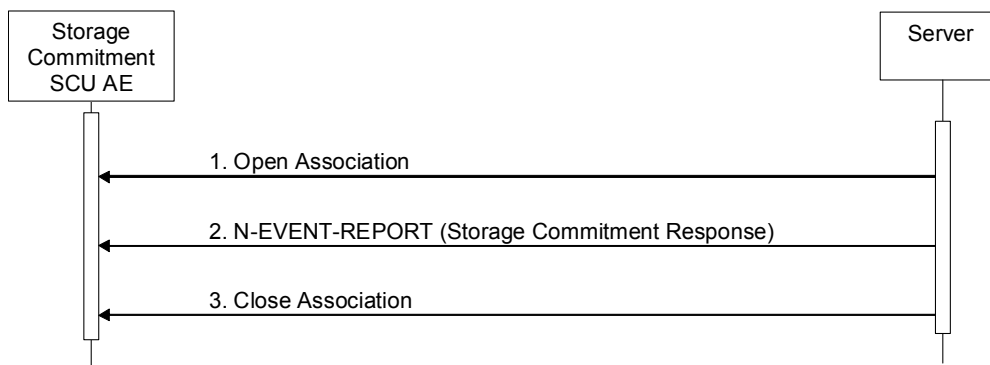


Figure 4.2-3
SEQUENCING OF ACTIVITY - RECEIVE STORAGE COMMITMENT RESPONSE

A possible sequence of interactions between the Storage Commitment SCU AE and a Server (e.g. a storage or archive device supporting Storage Commitment SOP Classes as an SCP) is illustrated in the Figure above:

1. The Server opens an association with the Storage Commitment SCU AE.
2. The Server sends an N-EVENT-REPORT request notifying the Storage SCU AE of the status of a previous storage commitment request. The Storage SCU AE replies with an N-EVENT-REPORT response confirming receipt.
3. The Server closes the association with the Storage Commitment SCU AE.

The Storage Commitment SCU AE may reject association attempts as shown in the table below. The Result, Source and Reason/Diag columns represent the values returned in the appropriate fields of an ASSOCIATE-RJ PDU (see PS3.8, Section 9.3.4).

Table 4.2-18
ASSOCIATION REJECTION REASONS

Result	Source	Reason/Diag	Explanation
1 – rejected-permanent	DICOM UL service-user	3 – calling-AE-title-not-recognized	The association request contained an unrecognized calling AE Title. An association request with the same parameters will not succeed at a later time unless configuration changes are made. This rejection reason normally occurs when the association acceptor has not been configured to recognize the AE Title of the association initiator.
1 – rejected-permanent	DICOM UL service-provider (ASCE related function)	1 – no-reason-given	The association request could not be parsed. An association request with the same format will not succeed at a later time.

4.2.2.4.1.2 Accepted Presentation Contexts

The Storage Commitment SCU AE will accept Presentation Contexts shown in the table below.

**Table 4.2-19
ACCEPTABLE PRESENTATION CONTEXTS FOR
ACTIVITY RECEIVE STORAGE COMMITMENT RESPONSE**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.2.4.1.3 SOP Specific Conformance for Storage Commitment SOP Class

4.2.2.4.1.3.1 Storage Commitment Notifications (N-EVENT-REPORT)

The Storage Commitment SCU AE provides standard conformance to the Storage Commitment Service Class as an SCU.

The behavior of Storage Commitment SCU AE when receiving Event Types within the N-EVENT-REPORT is summarized in the table below.

**Table 4.2-20
STORAGE COMMITMENT N-EVENT-REPORT BEHAVIOUR**

Event Type Name	Event Type ID	Behavior
Storage Commitment Request Successful	1	The Storage Commitment SCU AE permits the operator(s) to delete the Referenced SOP Instances under Referenced SOP Sequence (0018,1199), or deletes the Instances from the local database automatically.
Storage Commitment Request Complete – Failures Exist	2	The Storage Commitment SCU AE requests the Storage SCU AE to send the Referenced SOP Instances under Failed SOP Sequence (0018,1198).

The reasons for returning specific status codes in a N-EVENT-REPORT response are summarized in the table below.

**Table 4.2-21
STORAGE COMMITMENT N-EVENT-REPORT RESPONSE STATUS REASONS**

Service Status	Further Meaning	Status Code	Reasons
Success	Success	0000	The storage commitment result has been successfully received.
Failure	Processing Failure	0110H	An internal error occurred during processing of the N-EVENT-REPORT. A short description of the error will be returned in Error Comment (0000,0902).

4.2.3 MWM SCU AE Specification

4.2.3.1 SOP Classes

The MWM SCU AE provides Standard Conformance to the following SOP Classes:

Table 4.2-22
SOP CLASSES FOR THE MWM SCU AE

SOP Class Name	SOP Class UID	SCU	SCP
Modality Worklist Information Model – FIND	1.2.840.10008.5.1.4.31	Yes	No

4.2.3.2 Association Policies

4.2.3.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

Table 4.2-23
DICOM APPLICATION CONTEXT FOR THE MWM SCU AE

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

4.2.3.2.2 Number of Associations

The MWM SCU AE initiates one association at a time for a worklist request.

Table 4.2-24
NUMBER OF ASSOCIATIONS INITIATED FOR THE MWM SCU AE

Maximum number of simultaneous associations	1
---	---

4.2.3.2.3 Asynchronous Nature

The MWM SCU AE does not support asynchronous communication (multiple outstanding transactions over a single association).

Table 4.2-25
ASYNCHRONOUS NATURE FOR THE MWM SCU AE

Maximum number of outstanding asynchronous transactions	1
---	---

4.2.3.2.4 Implementation Identifying Information

The implementation information for this Application Entity is:

Table 4.2-26
DICOM IMPLEMENTATION CLASS AND VERSION FOR THE MWM SCU AE

Implementation Class UID	1.2.392.200036.9116.6.15.1000.1
Implementation Version Name	TM_ARTIDA_1.0

4.2.3.3 Association Initiation Policy

4.2.3.3.1 Activity – Update Worklist

4.2.3.3.1.1 Description and Sequencing of Activities

The request for an “Update Worklist” is initiated by user interaction, i.e. pressing the buttons “Get Worklist” or automatically at the time of patient registration.

Upon initiation of the request, the MWM SCU AE will build an Identifier for the C-FIND request, will initiate an association to send the request and will wait for worklist responses. After retrieval of all responses, the MWM SCU AE will access the local database to add or update patient demographic data. The results will be displayed in a separate list.

The MWM SCU AE will initiate an association in order to issue a C-FIND request according to the Modality Worklist Information Model.

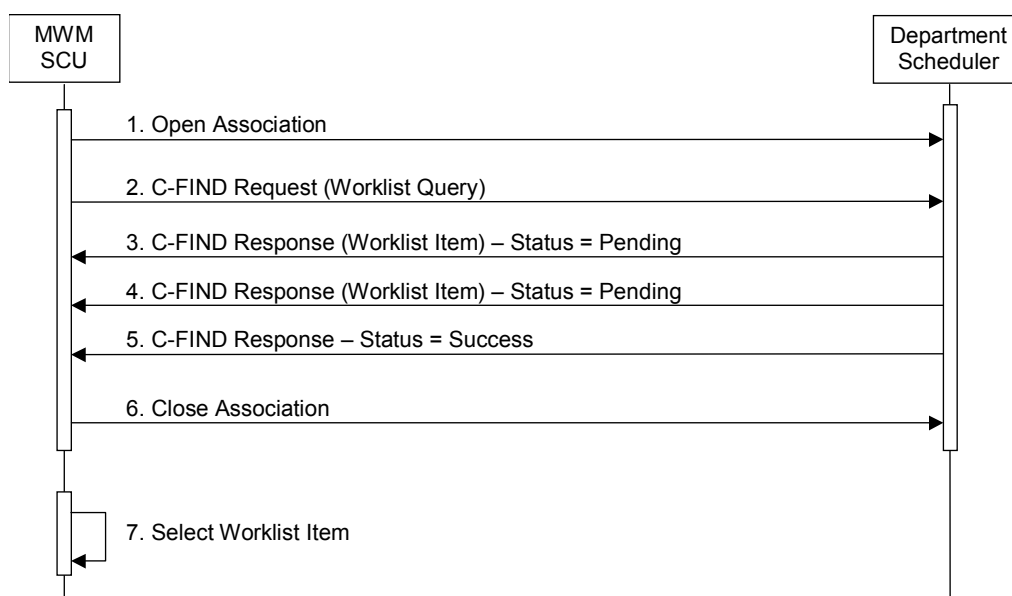


Figure 4.2-4
SEQUENCING OF ACTIVITY – UPDATE WORKLIST

A possible sequence of interactions between the MWM SCU AE and a Department Scheduler (e.g. a device such as a RIS or HIS which supports the Modality Worklist SOP Class as an SCP) is illustrated in the Figure above:

1. The MWM SCU AE opens an association with the Department Scheduler
2. The MWM SCU AE sends a C-FIND request to the Department Scheduler containing the Worklist Query attributes.
3. The Department Scheduler returns a C-FIND response containing the requested attributes of the first matching worklist item.
4. The Department Scheduler returns another C-FIND response containing the requested attributes of the second matching worklist item.
5. The Department Scheduler returns another C-FIND response with status Success indicating that no further matching worklist items exist. This example assumes that only 2 worklist items match the Worklist Query.
6. The MWM SCU AE closes the association with the Department Scheduler.
7. The user selects a worklist item from the Worklist and prepares to acquire new instances.

4.2.3.3.1.2 Proposed Presentation Contexts

The MWM SCU AE will propose Presentation Contexts shown in the following table:

**Table 4.2-27
PROPOSED PRESENTATION CONTEXTS FOR ACTIVITY UPDATE WORKLIST**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Modality Worklist Information Model – FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.3.3.1.3 SOP Specific Conformance for Modality Worklist SOP Class

The MWM SCU AE provides standard conformance to the Modality Worklist SOP Class as an SCU.

The behavior of the MWM SCU when encountering status codes in a Modality Worklist C-FIND response is summarized in the table below.

**Table 4.2-28
MODALITY WORKLIST C-FIND RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Status Code	Behavior
Success	Matching is complete	0000	The SCP has completed the matches. Worklist items are available for display or further processing.
*	*	Any other status code	The association is aborted using A-ABORT and the status meaning is logged.

The behavior of the MWM SCU AE during communication failure is summarized in the table below.

**Table 4.2-29
MODALITY WORKLIST COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	The association is aborted using A-ABORT and the reason is logged.
Unsupported character sets	
Association aborted by the SCP or network layers	The reason is logged.

Acquired instances will always use the Study Instance UID specified for the Scheduled Procedure Step (if available). If an acquisition is unscheduled, a Study Instance UID will be generated locally.

The table below provides a description of the MWM SCU AE Worklist Request Identifier and specifies the attributes that are copied into the instances. Unexpected attributes returned in a C-FIND response are ignored.

Table 4.2-30
WORKLIST REQUEST IDENTIFIER

Module Name Attribute Name	Tag	VR	M	R	D	IOD
SOP Common						
Specific Character Set	(0008,0005)	CS				x
Scheduled Procedure Step						
Scheduled Procedure Step Sequence	(0040,0100)	SQ				x
>Modality	(0008,0060)	CS	S	x	x	x
>Requested Contrast Agent	(0032,1070)	LO		x		
>Scheduled Station AE Title	(0040,0001)	AE	S	x	x	x
>Scheduled Procedure Step Start Date	(0040,0002)	DA	R		x	x
>Scheduled Procedure Step Start Time	(0040,0003)	TM	R		x	x
>Scheduled Performing Physician's Name	(0040,0006)	PN		x	x	x
>Scheduled Procedure Step Description	(0040,0007)	LO		x	x	x
>Scheduled Station Name	(0040,0010)	SH		x		
>Scheduled Procedure Step Location	(0040,0011)	SH		x		
>Scheduled Protocol Code Sequence	(0040,0008)	SQ				x
>>Code Value	(0008,0100)	SH		x	x	x
>>Coding Scheme Designator	(0008,0102)	SH		x	x	x
>>Coding Scheme Version	(0008,0103)	SH		x	x	x
>>Code Meaning	(0008,0104)	LO		x	x	x
>Pre-Medication	(0040,0012)	LO		x		
>Scheduled Procedure Step Status	(0040,0020)	CS		x		
>Scheduled Procedure Step ID	(0040,0009)	SH		x	x	x
Requested Procedure						
Referenced Study Sequence	(0008,1110)	SQ				x
>Referenced SOP Class UID	(0008,1150)	UI		x		x
>Referenced SOP Instance UID	(0008,1155)	UI		x		x
Study Instance UID	(0020,000D)	UI		x		x
Requested Procedure Description	(0032,1060)	LO		x	x	x
Requested Procedure Code Sequence	(0032,1064)	SQ				x
>Code Value	(0008,0100)	SH		x		x
>Coding Scheme Designator	(0008,0102)	SH		x		x
>Coding Scheme Version	(0008,0103)	SH		x		x
>Code Meaning	(0008,0104)	LO		x		x
Requested Procedure ID	(0040,1001)	SH	S	x	x	x
Requested Procedure Priority	(0040,1003)	SH		x		
Patient Transport Arrangements	(0040,1004)	LO		x		
Imaging Service Request						
Accession Number	(0008,0050)	SH	S	x	x	x
Referring Physician's Name	(0008,0090)	PN		x	x	x
Requesting Physician	(0032,1032)	PN		x	x	x
Visit Identification						
Admission ID	(0038,0010)	LO		x		
Visit Status						
Current Patient Location	(0038,0300)	LO		x		
Patient's Institution Residence	(0038,0400)	LO		x	x	
Visit Relationship						
Referenced Patient Sequence	(0008,1120)	SQ				
>Referenced SOP Class UID	(0008,1150)	UI		x		
>Referenced SOP Instance UID	(0008,1155)	UI		x		

Patient Identification						
Patient's Name	(0010,0010)	PN	W	x	x	x
Patient ID	(0010,0020)	LO	S	x	x	x
Patient Demographic						
Patient's Birth Date	(0010,0030)	DA		x	x	x
Patient's Sex	(0010,0040)	CS		x	x	x
Patient's Size	(0010,1020)	DS		x	x	x
Patient's Weight	(0010,1030)	DS		x	x	x
Patient Comments	(0010,4000)	LT		x	x	x
Confidentiality constraint on patient data	(0040,3001)	LO		x		x
Patient Medical						
Medical Alerts	(0010,2000)	LO		x		x
Allergies	(0010,2110)	LO		x		x
Pregnancy Status	(0010,21C0)	US		x		x
Special Needs	(0038,0050)	LO		x		x
Patient State	(0038,0500)	LO		x		x
Other Attributes						
Study Description	(0008,1030)	LO		x	x	x

The above table should be read as follows:

- Module Name: The name of the associated module for supported worklist attributes.
- Attribute Name: Attributes supported to build the MWM SCU AE Worklist Request Identifier.
- Tag: DICOM tag for this attribute.
- VR: DICOM VR for this attribute.
- M: Matching keys for (automatic) Worklist Update.
S: Single Value Matching
R: Range Matching
W: Wild Card Matching
- R: Return keys. An "x" will indicate that the MWM SCU AE will supply this attribute as Return Key with zero length for Universal Matching. This setting can be configured using the service tool.
- D: Displayed keys. An "x" indicates that this worklist attribute is displayed to the user during a patient registration. For example, Patient Name will be displayed when registering the patient prior to an examination.
- IOD: An "x" indicates that this worklist attribute is included into all Object Instances created during performance of the related Procedure Step.

Notes: Specific Character Set (0008,0005) will be created if an extended or replacement character set is used in the matching keys.

Scheduled Performing Physician's Name (0040,1006) will be copied into Performing Physician's Name (0008,1050).

Patient's Institution Residence (0038,0400) will be displayed as *In Patient* or *Out Patient* when matching the following string: Inpatient or Outpatient.

In the default setting, Study Description (0008,1030) will be displayed at *Exam Type* when matching the following exam types: Adult Heart, Pediatric Heart, Coronary, M-TEE, PV Arterial, PV Venous, Carotid, Digits, or OTHER. They can be also configured to correspond to user-defined terms, and it is selectable where to set those terms: Study Description (0008,1030), Scheduled Procedure Step Description (0040,0007), or Requested Procedure Description (0032,1060).

4.2.3.4 Association Acceptance Policy

The MWM SCU AE does not accept associations.

4.2.4 MPPS SCU AE Specification

4.2.4.1 SOP Classes

The MPPS SCU AE provides Standard Conformance to the following SOP Classes:

Table 4.2-31
SOP CLASSES FOR THE MPPS SCU AE

SOP Class Name	SOP Class UID	SCU	SCP
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Yes	No

4.2.4.2 Association Policies

4.2.4.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

Table 4.2-32
DICOM APPLICATION CONTEXT FOR THE MPPS SCU AE

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

4.2.4.2.2 Number of Associations

The MPPS SCU AE initiates one association at a time.

Table 4.2-33
NUMBER OF ASSOCIATIONS INITIATED FOR THE MPPS SCU AE

Maximum number of simultaneous associations	1
---	---

4.2.4.2.3 Asynchronous Nature

The MPPS SCU AE does not support asynchronous communication (multiple outstanding transactions over a single association).

Table 4.2-34
ASYNCHRONOUS NATURE FOR THE MPPS SCU AE

Maximum number of outstanding asynchronous transactions	1
---	---

4.2.4.2.4 Implementation Identifying Information

The implementation information for this Application Entity is:

Table 4.2-35
DICOM IMPLEMENTATION CLASS AND VERSION FOR THE MPPS SCU AE

Implementation Class UID	1.2.392.200036.9116.6.15.1000.1
Implementation Version Name	TM_ARTIDA_1.0

4.2.4.3 Association Initiation Policy

4.2.4.3.1 Activity – Acquire Instances

4.2.4.3.1.1 Description and Sequencing of Activities

The MPPS SCU AE performs the creation of an MPPS instance automatically when the user selects and starts a worklist item. Further updates on the MPPS data can be performed when the user completes the acquisition.

The MPPS SCU AE will initiate an association to issue an:

- N-CREATE request according to the CREATE Modality Performed Procedure Step SOP Instance operation, or an:
- N-SET request to update the contents and state of the MPPS according to the SET Modality Performed Procedure Step Information operation.

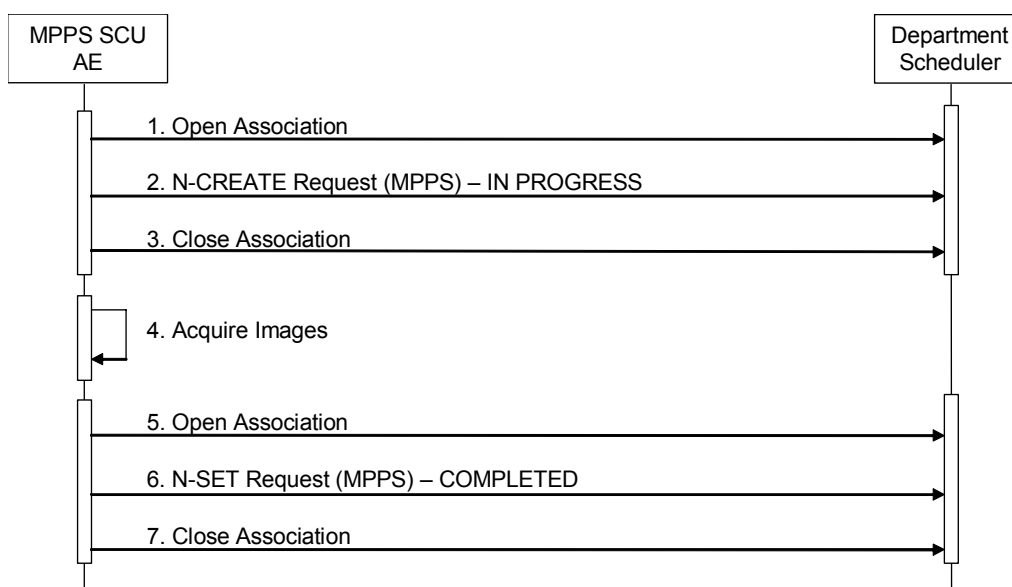


Figure 4.2-5
SEQUENCING OF ACTIVITY – ACQUIRE INSTANCES

A possible sequence of interactions between the MPPS SCU AE and a Department Scheduler (e.g. a device such as a RIS or HIS which supports the MPPS SOP Class as an SCP) is illustrated in the Figure above:

1. The MPPS SCU AE opens an association with the Department Scheduler
2. The MPPS SCU AE sends an N-CREATE request to the Department Scheduler to create an MPPS instance with status of “IN PROGRESS” and create all necessary attributes. The Department Scheduler acknowledges the MPPS creation with an N-CREATE response (status success).
3. The MPPS SCU AE closes the association with the Department Scheduler.
4. All instances are acquired and stored in the local database.
5. The MPPS SCU AE opens an association with the Department Scheduler.
6. The MPPS SCU AE sends an N-SET request to the Department Scheduler to update the MPPS instance with status of “COMPLETED” and set all necessary attributes. The Department Scheduler acknowledges the MPPS update with an N-SET response (status success).
7. The MPPS SCU AE closes the association with the Department Scheduler.

4.2.4.3.1.2 Proposed Presentation Contexts

The MPPS SCU AE will propose Presentation Contexts shown in the following table:

**Table 4.2-36
PROPOSED PRESENTATION CONTEXTS FOR REAL-WORLD ACTIVITY ACQUIRE INSTANCES**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.4.3.1.3 SOP Specific Conformance for MPPS SOP Class

The MPPS SCU AE provides standard conformance to the Modality Performed Procedure Step SOP Class as an SCU.

The behavior of the MPPS SCU AE when encountering status codes in an MPPS N-CREATE or N-SET response is summarized in the table below.

**Table 4.2-37
MPPS N-CREATE / N-SET RESPONSE STATUS HANDLING BEHAVIOR**

Service Status	Further Meaning	Status Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
*	*	Any other status code	The association is aborted and the MPPS is marked as failed. The status meaning is logged and reported to the user.

The behavior of the MPPS SCU AE during communication failure is summarized in the table below:

**Table 4.2-38
MPPS COMMUNICATION FAILURE BEHAVIOR**

Exception	Behavior
Timeout	The association is aborted and MPPS is marked as failed. The reason is logged and reported to the user.
Association aborted by the SCP or network layers	The MPPS is marked as failed. The reason is logged and reported to the user.

The table below provides a description of the MPPS N-CREATE and N-SET request identifiers sent by the MPPS SCU AE. Empty cells in the N-CREATE and N-SET columns indicate that the attribute is not sent. An "x" indicates that an appropriate value will be sent. A "Zero length" attribute will be sent with zero length.

**Table 4.2-39
MPPS N-CREATE / N-SET REQUEST IDENTIFIER**

Attribute Name	Tag	VR	N-CREATE	N-SET
Specific Character Set	(0008,0005)	CS	Created, if an extended or replacement character set is used.	
Performed Procedure Step Relationship				
Scheduled Step Attributes Sequence	(0040,0270)	SQ	Always set	
>Study Instance UID	(0020,000D)	UI	From Modality Worklist	
>Referenced Study Sequence	(0008,1110)	SQ	From Modality Worklist	
>>Referenced SOP Class UID	(0008,1150)	UI	From Modality Worklist	
>>Referenced SOP Instance UID	(0008,1155)	UI	From Modality Worklist	
>Accession Number	(0008,0050)	SH	From Modality Worklist	
>Placer Order Number/Imaging Service Request	(0040,2016)	LO	Zero length	
>Filler Order Number/Imaging Service Request	(0040,2017)	LO	Zero length	
>Requested Procedure ID	(0040,1001)	SH	From Modality Worklist	
>Requested Procedure Description	(0032,1060)	LO	From Modality Worklist	
>Scheduled Procedure Step ID	(0040,0009)	SH	From Modality Worklist	
>Scheduled Procedure Step Description	(0040,0007)	LO	From Modality Worklist	
>Scheduled Protocol Code Sequence	(0040,0008)	SQ	From Modality Worklist	
Patient's Name	(0010,0010)	PN	From Modality Worklist or user input	
Patient ID	(0010,0020)	LO	From Modality Worklist or user input	
Patient's Birth Date	(0010,0030)	DA	From Modality Worklist or user input	
Patient's Sex	(0010,0040)	CS	From Modality Worklist or user input	
Referenced Patient Sequence	(0008,1120)	SQ	From Modality Worklist	
>Referenced SOP Class UID	(0008,1150)	UI	From Modality Worklist	
>Referenced SOP Instance UID	(0008,1155)	UI	From Modality Worklist	
Performed Procedure Step Information				
Performed Procedure Step ID	(0040,0253)	SH	x	
Performed Station AE Title	(0040,0241)	AE	MPPS AE Title	
Performed Station Name	(0040,0242)	SH	From configuration	
Performed Location	(0040,0243)	SH	Zero length	
Performed Procedure Step Start Date	(0040,0244)	DA	Actual start date	
Performed Procedure Step Start Time	(0040,0245)	TM	Actual start time	
Performed Procedure Step Status	(0040,0252)	CS	IN PROGRESS	COMPLETED or DISCONTINUED
Performed Procedure Step Description	(0040,0254)	LO	x	
Performed Procedure Type Description	(0040,0255)	LO	Zero length	
Procedure Code Sequence	(0008,1032)	SQ	Zero or more items	Zero or more items
Performed Procedure Step End Date	(0040,0250)	DA	Zero length	Actual end date
Performed Procedure Step End Time	(0040,0251)	TM	Zero length	Actual end time
Image Acquisition Results				
Modality	(0008,0060)	CS	US	
Study ID	(0020,0010)	SH	x	

Performed Protocol Code Sequence	(0040,0260)	SQ	Zero or more items	Zero or more items
Performed Series Sequence	(0040,0340)	SQ	One or more items	One or more items
>Performing Physician's Name	(0008,1050)	PN	From Modality Worklist or user input	x
>Protocol Name	(0018,1030)	LO	x	x
>Operator's Name	(0008,1070)	PN	Zero length	Zero length
>Series Instance UID	(0020,000E)	UI	x	x
>Series Description	(0008,103E)	LO	Zero length	Zero length
>Retrieve AE Title	(0008,0054)	AE	Zero length	Zero length
>Referenced Image Sequence	(0008,1140)	SQ	Zero or more items	One or more items
>>Referenced SOP Class UID	(0008,1150)	UI	x	x
>>Referenced SOP Instance UID	(0008,1155)	UI	x	x
>Referenced Non-Image Composite SOP Instance Sequence	(0040,0220)	SQ	Zero length	Zero length

4.2.4.4 Association Acceptance Policy

The MPPS SCU AE does not accept associations.

4.2.5 Storage SCP AE Specification

4.2.5.1 SOP Classes

The Storage SCP AE provides Standard Conformance to the following SOP Classes:

Table 4.2-40
SOP CLASSES FOR THE STORAGE SCP AE

SOP Class Name	SOP Class UID	SCU	SCP
Verification	1.2.840.10008.1.1	No	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7		
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1		
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1		
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22		

4.2.5.2 Association Policies

4.2.5.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

Table 4.2-41
DICOM APPLICATION CONTEXT FOR THE STORAGE SCP AE

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

4.2.5.2.2 Number of Associations

The Storage SCP AE can support up to seven associations at a time.

Table 4.2-42
NUMBER OF ASSOCIATIONS ACCEPTED FOR THE STORAGE SCP AE

Maximum number of simultaneous associations	10
---	----

4.2.5.2.3 Asynchronous Nature

The Storage SCP AE does not support asynchronous communication (multiple outstanding transactions over a single association).

Table 4.2-43
ASYNCHRONOUS NATURE FOR THE STORAGE SCP AE

Maximum number of outstanding asynchronous transactions	1
---	---

4.2.5.2.4 Implementation Identifying Information

The implementation information for the Storage SCP AE is:

Table 4.2-44
DICOM IMPLEMENTATION CLASS AND VERSION FOR THE STORAGE SCP AE

Implementation Class UID	1.2.392.200036.9116.6.15.1000.1
Implementation Version Name	TM_ARTIDA_1.0

4.2.5.3 Association Initiation Policy

The Storage SCP AE does not initiate associations.

4.2.5.4 Association Acceptance Policy

The Storage SCP AE accepts associations only if they have valid Presentation Contexts. If none of the requested Presentation Contexts are accepted then the association request itself is rejected. It can be configured to only accept associations with certain hosts (using TCP/IP address) and/or AE Titles.

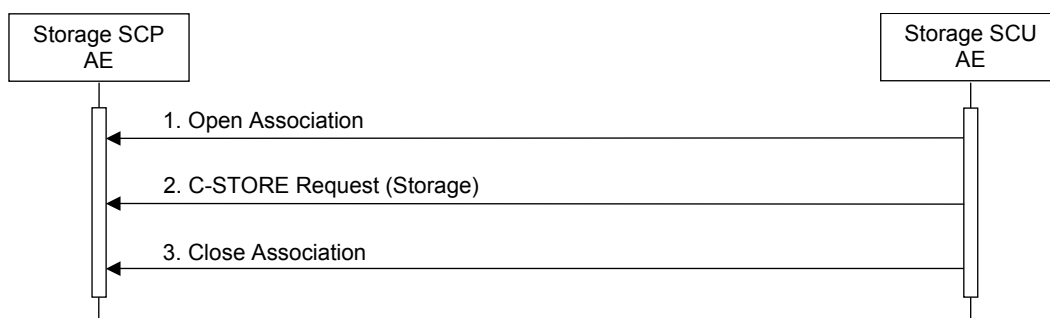


Figure 4.2-6
SEQUENCING OF ACTIVITY – STORE IMAGES TO THE LOCAL FILE SYSTEM

A possible sequence of interactions between the Storage SCP AE and a Storage SCU AE is illustrated in the Figure above:

1. The Storage SCU AE opens an association with the Storage SCP AE.
2. The Storage SCU AE sends images to the Storage SCP AE using a storage request (C-STORE) and the Storage SCP AE replies with a C-STORE response (status success).
3. The Storage SCU AE closes the association with the Storage SCP AE.

The Storage SCP AE may reject association attempts as shown in the Table 4.2-18.

4.2.5.4.1.1 Accepted Presentation Contexts

The default behavior of the Storage SCP AE supports the Implicit VR Little Endian and Explicit VR Little Endian transfer syntaxes. If the both transfer syntaxes are proposed per presentation context then the Storage SCP AE will select Explicit VR Little Endian Transfer Syntax.

Any of the presentation contexts shown in the following table are acceptable to the Storage SCP AE.

**Table 4.2-45
ACCEPTED PRESENTATION CONTEXTS BY THE STORAGE SCP AE**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50		
		JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian	1.2.840.10008.1.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50		
		JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50		
		JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Implicit VR Little Endian	1.2.840.10008.1.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

4.2.5.4.1.2 SOP Specific Conformance for Storage SOP Classes

The associated Activity with the Storage service is the storage of medical data received over the network on a designated hard disk. The Storage SCP AE will return a failure status if it is unable to store the instances on to the hard disk.

The Storage SCP AE is Level 0 conformant as a Storage SCP.

Table 4.2-46
THE STORAGE SCP AE C-STORE RESPONSE STATUS RETURN REASONS

Service Status	Further Meaning	Status Code	Reason
Success	Success	0000	The Composite SOP Instance was successfully received, verified, and stored in the system database.
Refused	Out of Resources	A700	Indicates that there was not enough local resources.
Error	Cannot Understand	C000	Indicates that the Storage SCP AE cannot parse the Data Set into Elements. (e.g. when receiving unsupported character sets)

4.3 NETWORK INTERFACES

4.3.1 Physical Network Interface

This product supports a single network interface. One of the following physical network interfaces will be available depending on installed hardware options:

Table 4.3-1
SUPPORTED PHYSICAL NETWORK INTERFACES

Ethernet 1000baseT
Ethernet 100baseT
Ethernet 10baseT

4.3.2 Additional Protocols

None.

4.4 CONFIGURATION

4.4.1 AE Title/Presentation Address Mapping

4.4.1.1 Local AE Titles

All local applications use the AE Titles and TCP/IP Ports configured via the service tool. The Field Service Engineer can configure the TCP Port via the service tool.

Note: Up to 16 characters (alphanumeric characters, "-", ".", and "_") can be used in the AE Titles.

**Table 4.4-1
AE TITLE CONFIGURATION TABLE**

Application Entity	Default AE Title	Default TCP/IP Port
MWM SCU	MWMSCU_AE	Not Applicable
MPPS SCU	MPPSSCU_AE	
Storage SCU	DICOM_LOCAL_SCU	
Storage SCP	DICOM_LOCAL_SCP	104
Storage Commitment SCU		

4.4.1.2 Remote AE Title/Presentation Address Mapping

The AE Titles, host names and port numbers of remote applications are configured using the service tool.

Note: Up to 16 characters (alphanumeric characters, "-", ".", and "_") can be used in the AE Titles.

4.4.2 Parameters

A large number of parameters related to acquisition and general operation can be configured using the service tool. The table below only shows those configuration parameters relevant to DICOM communication. See the Product's Service Manual for details on general configuration capabilities.

**Table 4.4-2
CONFIGURATION PARAMETERS TABLE**

Parameter	Configurable (Yes/No)	Default Value
General Parameters		
Maximum PDU send/receive size	Yes	28 Kbytes
Time-out waiting for an acceptance or rejection response to an association request (Application Level Timeout)	No	240 sec
Time-out waiting for a response to an association release request (Application Level Timeout)	No	240 sec
Time-out waiting for completion of a TCP/IP connect request (Low-level timeout)	No	240 sec
Time-out awaiting a response to a DIMSE request (Low-Level Timeout)	No	240 sec
Time-out for waiting for data between TCP/IP-packets (Low Level Timeout)	No	240 sec

Parameter	Configurable (Yes/No)	Default Value
Storage SCU Parameters		
Maximum number of simultaneously initiated associations by the Storage SCU AE	No	10
Number of times a failed send job may be retried	No	Forever, until the job succeeds or user cancels it.
Storage Commitment SCU Parameters		
Maximum number of simultaneously initiated associations by the Storage Commitment SCU AE	No	10
Maximum number of simultaneously accepted associations by the Storage Commitment SCU AE	No	10
Time-out waiting for a Storage Commitment Notification (maximum duration of applicability for a Storage Commitment Transaction UID)	Yes	180 sec
Delay association release after sending a storage commitment request (wait for a storage commitment notification over the same association)	No	0
Modality Worklist SCU Parameters		
Maximum number of simultaneously initiated associations by the MWM SCU AE	No	1
Modality Worklist SCU time-out waiting for the final response to a C-FIND-RQ	Yes	60 sec
Maximum number of worklist items	Yes	200
Query worklist for specific Scheduled Station AE Title	Yes	MWMSCU_AE
Query worklist for specific Modality	Yes	US
MPPS SCU Parameters		
Maximum number of simultaneously initiated associations by the MPPS SCU AE	No	1
Number of times a failed send job may be retried	No	Forever, until the job succeeds or user cancels it.
Storage SCP Parameters		
Maximum number of simultaneously initiated associations by the Storage SCP AE	No	10

5. MEDIA INTERCHANGE

5.1 IMPLEMENTATION MODEL

5.1.1 Application Data Flow

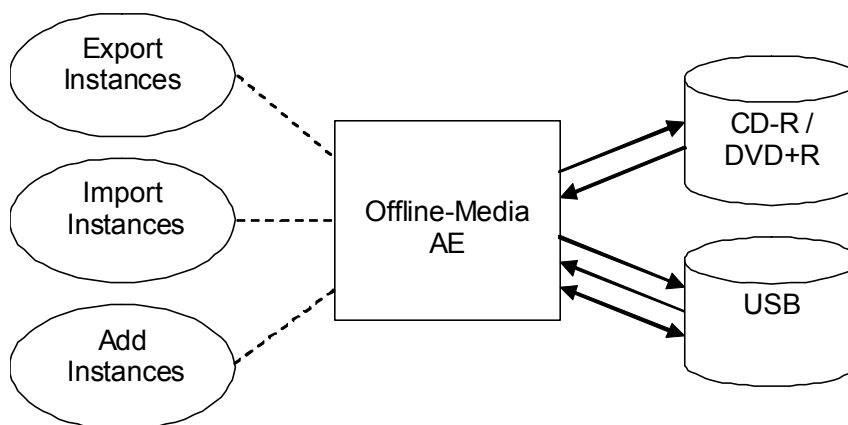


Figure 5.1-1
APPLICATION DATA FLOW DIAGRAM FOR MEDIA STORAGE

- The Offline-Media AE exports instances to a CD-R, DVD+R or USB Storage medium. It is associated with the local real-world activity “Export Instances” performed upon user request.
- The Offline-Media AE imports instances from a CD-R, DVD+R or USB Storage medium. It is associated with the local real-world activity “Import Instances” performed upon user request.
- The Offline-Media AE updates instances from a USB Storage medium. It is associated with the local real-world activity “Add Instances” performed upon user request.

5.1.2 Functional Definition of AEs

5.1.2.1 Functional Definition of Offline-Media AE

The Offline-Media AE is performed upon user request for selected instances to/from an offline DICOM CD-R, DVD+R or USB medium. It therefore performs the following tasks:

Export:

- Builds DICOM Information Objects.
- Creates a DICOMDIR file that represents the contents of the DICOM Information Objects to be recorded.
- Records DICOM Information Objects and the DICOMDIR file to the CD-R, DVD+R or USB medium.

Import:

- Reads the DICOMDIR file that represents the contents of the data as recorded.
- Displays the ordered list of instances, identifying information.
- Loads the selected instances from the CD-R, DVD+R or USB medium and displays them on the screen.

Addition:

- Reads a File-set of the USB medium and writes it to the local storage device.
- Adds the instances to the File-set, then writes it to the medium.
- Modifies the DICOMDIR file.

Note: The Offline-Media AE can update files created by the product itself.

5.1.3 Sequencing of Real-World Activities

5.1.3.1 Activity – Export Instances

Operator requests to create new File-set(s) onto a new CD-R, DVD+R or USB medium. The requests are placed in a queue and are executed in the background.

The operations for “Export Instances” are described below:

- Step-1: Select the instances on the local storage device to be created to the medium.
- Step-2: Request to copy to the medium.

5.1.3.2 Activity – Import Instances

Operator requests to retrieve File-set(s) on the CD-R, DVD+R or USB medium. The requests are placed in a queue and are executed in the background.

The operations for “Import Instances” are described below:

- Step-1: Select the instances on the medium to be retrieved to the local storage device.
- Step-2: Request to copy to the local storage device.

5.1.3.3 Activity – Add Instances

Operator requests to add new objects to an already existing File-set on the USB medium. The requests are placed in a queue and are executed in the background.

The operations for “Add Instances” are described below:

- Step-1: Select the instances on the local storage device to be added to the medium.
- Step-2: Request to copy to the medium.

5.1.4 File Meta Information for Implementation Class and Version

The implementation information written to the File Meta Header in each file is:

**Table 5.1-1
DICOM IMPLEMENTATION CLASS AND VERSION FOR MEDIA STORAGE**

File Meta Information Version	1
Implementation Class UID	1.2.392.200036.9116.6.15.1000.1
Implementation Version Name	TM_ARTIDA_1.0

5.2 AE SPECIFICATIONS

5.2.1 Offline-Media AE Specification

The Offline-Media AE provides standard conformance to the DICOM Interchange Option of the Media Storage Service Class. The Application Profiles and roles are listed below:

**Table 5.2-1
APPLICATION PROFILES, ACTIVITIES AND ROLES FOR OFFLINE-MEDIA**

Application Profiles Supported	Real World Activity	Role	SC Option
AUG-GEN-CD, AUG-GEN-DVD	Export Instances	FSC	Interchange
	Import Instances	FSR	Interchange
AUG-GEN-USB	Export Instances	FSC	Interchange
	Import Instances	FSR	Interchange
	Add Instances	FSU	Interchange

5.2.1.1 File Meta Information for the Application Entity

The Source Application Entity Title is the local AE title of Storage SCP.

5.2.1.2 Real-World Activities

5.2.1.2.1 Activity – Export Instances

The Offline-Media AE acts as an FSC using the interchange option when requested to export SOP Instances from the local database to a CD-R, DVD+R or USB medium.

5.2.1.2.1.1 Media Storage Application Profiles

The Offline-Media AE supports the AUG-GEN-CD, AUG-GEN-DVD and AUG-GEN-USB Application Profiles.

5.2.1.2.1.1.1 Options

The Offline-Media AE supports the SOP Classes and Transfer Syntaxes listed in Table 5.3-1.

5.2.1.2.2 Activity – Import Instances

The Offline-Media AE acts as an FSR using the interchange option when requested to import SOP Instances from a CD-R, DVD+R or USB medium to the local database.

5.2.1.2.2.1 Media Storage Application Profiles

The Offline-Media AE supports the AUG-GEN-CD, AUG-GEN-DVD and AUG-GEN-USB Application Profiles.

5.2.1.2.2.1.1 Options

The Offline-Media AE supports the SOP Classes and Transfer Syntaxes listed in Table 5.3-1..

5.2.1.2.3 Activity – Add Instances

The Offline-Media AE acts as an FSU using the interchange option when requested to add SOP Instances from the local database to a USB medium.

5.2.1.2.3.1 Media Storage Application Profiles

The Offline-Media AE supports the AUG-GEN-USB Application Profiles.

5.2.1.2.3.1.1 Options

The Offline-Media AE supports the SOP Classes and Transfer Syntaxes listed in Table 5.3-1.

5.3 AUGMENTED AND PRIVATE APPLICATION PROFILES

5.3.1 Augmented Application Profiles

5.3.1.1 Augmented Application Profiles

– AUG-GEN-CD, AUG-GEN-DVD and AUG-GEN-USB

5.3.1.1.1 SOP Class Augmentations

The Augmented Application Profiles support the following SOP Classes and Transfer Syntaxes:

**Table 5.3-1
SOP CLASS AUGMENTATIONS**

Information Object Definition	SOP Class UID	Transfer Syntax	Transfer Syntax UID
DICOM Media Storage Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian	1.2.840.10008.1.2.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian	1.2.840.10008.1.2.1
		JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70
		RLE Lossless	1.2.840.10008.1.2.5
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian	1.2.840.10008.1.2.1
		JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70
		RLE Lossless	1.2.840.10008.1.2.5
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian	1.2.840.10008.1.2.1
		JPEG Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossless, Non-Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70
		RLE Lossless	1.2.840.10008.1.2.5
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian	1.2.840.10008.1.2.1

5.3.1.1.2 Directory Augmentations

Not applicable.

5.3.1.1.3 Other Augmentations

Not applicable.

5.3.2 Private Application Profiles

Not applicable.

5.4 MEDIA CONFIGURATION

Not applicable.

6. SUPPORT OF CHARACTER SETS

This product supports ISO-IR 100 (Latin alphabet No.1) Supplementary set of ISO8859.

Notes: If the Storage SCP AE receives instances that contain characters from unsupported character sets, it will respond with "Cannot Understand" to the C-STORE request.

If the MWM SCU AE receives worklist items that contain characters from unsupported character sets, it may abort the association using A-ABORT.

7. SECURITY

This product does not support any specific security measures.

It is assumed that the product is used within a secured environment. It is assumed that a secured environment includes at a minimum:

- a. Firewall or router protections to ensure that only approved external hosts have network access to the product.
- b. Firewall or router protections to ensure that the product only has network access to approved external hosts and services.

Other network security procedures such as automated intrusion detection may be appropriate in some environments. Additional security features may be established by the local security policy and are beyond the scope of this conformance statement.

8. ANNEXES

8.1 IOD CONTENTS

8.1.1 Created SOP Instances

Table 8.1-1 specifies the attributes of a Secondary Capture Image transmitted by the Storage SCU AE.

Table 8.1-2 specifies the attributes of an Ultrasound Image transmitted by the Storage SCU AE.

Table 8.1-3 specifies the attributes of an Ultrasound Multi-frame Image transmitted by the Storage SCU AE.

Table 8.1-4 specifies the attributes of an Enhanced SR transmitted by the Storage SCU

The following tables use a number of abbreviations. The abbreviations used in the “Presence of ...” column are:

VNAP	Value Not Always Present (attribute sent zero length if no value is present)
ANAP	Attribute Not Always Present
ALWAYS	Always Present
EMPTY	Attribute is sent without a value

The abbreviations used in the “Source” column:

MWL	the attribute value source Modality Worklist
USER	the attribute value source is from user input
AUTO	the attribute value is generated automatically
MPPS	the attribute value is the same as that use for Modality Performed Procedure Step
CONFIG	the attribute value source is a configurable parameter

8.1.1.1 SC Image IOD

**Table 8.1-1
IOD OF CREATED SC IMAGE SOP INSTANCES**

IE	Module	Reference	Presence of Module
Patient	Patient	Table 8.1-5	ALWAYS
	Clinical Trial Subject	--	Not Present
Study	General Study	Table 8.1-6	ALWAYS
	Patient Study	Table 8.1-7	ALWAYS
	Clinical Trial Study	--	Not Present
Series	General Series	Table 8.1-8	ALWAYS
	Clinical Trial Series	--	Not Present
Equipment	General Equipment	Table 8.1-9	ALWAYS
	SC Equipment	Table 8.1-14	ALWAYS
Image	General Image	Table 8.1-10	ALWAYS
	Image Pixel	Table 8.1-11	ALWAYS
	SC Image	Table 8.1-15	Not Present
	Overlay Plane	--	Not Present
	Modality LUT	--	Not Present
	VOI LUT	--	Not Present
	SOP Common	Table 8.1-16	ALWAYS
	Private Application	Table 8.1-12	ALWAYS

8.1.1.2 US Image IOD

**Table 8.1-2
IOD OF CREATED US IMAGE SOP INSTANCES**

IE	Module	Reference	Presence of Module
Patient	Patient	Table 8.1-5	ALWAYS
	Clinical Trial Subject	--	Not Present
Study	General Study	Table 8.1-6	ALWAYS
	Patient Study	Table 8.1-7	ALWAYS
	Clinical Trial Study	--	Not Present
Series	General Series	Table 8.1-8	ALWAYS
	Clinical Trial Series	--	Not Present
Frame of Reference	Frame of Reference	--	Not Present
	Synchronization	--	Not Present
Equipment	General Equipment	Table 8.1-9	ALWAYS
Image	General Image	Table 8.1-10	ALWAYS
	Image Pixel	Table 8.1-11	ALWAYS
	Contrast/bolus	--	Not Present
	Palette Color Lookup Table	--	Not Present
	US Region Calibration	Table 8.1-13	ALWAYS
	US Image	Table 8.1-17	ALWAYS
	Overlay Plane	--	Not Present
	VOI LUT	--	Not Present
	SOP Common	Table 8.1-18	ALWAYS
	Private Application	Table 8.1-12	ALWAYS

8.1.1.3 US Multi-frame Image IOD

**Table 8.1-3
IOD OF CREATED US MULTI-FRAME IMAGE SOP INSTANCES**

IE	Module	Reference	Presence of Module
Patient	Patient	Table 8.1-5	ALWAYS
	Clinical Trial Subject	--	Not Present
Study	General Study	Table 8.1-6	ALWAYS
	Patient Study	Table 8.1-7	ALWAYS
	Clinical Trial Study	--	Not Present
Series	General Series	Table 8.1-8	ALWAYS
	Clinical Trial Series	--	Not Present
Frame of Reference	Frame of Reference	--	Not Present
	Synchronization	--	Not Present
Equipment	General Equipment	Table 8.1-9	ALWAYS
Image	General Image	Table 8.1-10	ALWAYS
	Image Pixel	Table 8.1-11	ALWAYS
	Contrast/bolus	--	Not Present
	Cine	Table 8.1-19	ALWAYS
	Multi-frame	Table 8.1-20	ALWAYS
	Frame Pointers	--	Not Present
	Palette Color Lookup Table	--	Not Present
	US Region Calibration	Table 8.1-13	ALWAYS
	US Image	Table 8.1-21	ALWAYS
	VOI LUT	--	Not Present
	SOP Common	Table 8.1-22	ALWAYS
	Private Application	Table 8.1-12	ALWAYS

8.1.1.4 Enhanced SR IOD

**Table 8.1-4
IOD OF CREATED ENHANCED SR SOP INSTANCES**

IE	Module	Reference	Presence of Module
Patient	Patient	Table 8.1-5	ALWAYS
	Specimen Identification	--	Not Present
	Clinical Trial Subject	--	Not Present
Study	General Study	Table 8.1-6	ALWAYS
	Patient Study	Table 8.1-7	ALWAYS
	Clinical Trial Study	--	Not Present
Series	SR Document Series	Table 8.1-23	ALWAYS
	Clinical Trial Series	--	Not Present
Equipment	General Equipment	Table 8.1-9	ALWAYS
Document	SR Document General	Table 8.1-24	ALWAYS
	SR Document Content	Table 8.1-25	ALWAYS
	SOP Common	Table 8.1-26	ALWAYS
	Private Application	Table 8.1-12	ALWAYS

8.1.1.5 Common Modules

**Table 8.1-5
PATIENT MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient's Name	(0010,0010)	PN		VNAP	MWL/ USER
Patient ID	(0010,0020)	LO		ALWAYS	MWL/ USER
Patient's Birth Date	(0010,0030)	DA	"18581118" will be entered if no value is present.	ALWAYS	MWL/ USER
Patient's Sex	(0010,0040)	CS		VNAP	MWL/ USER
Ethnic Group	(0010,2160)	SH		VNAP	MWL/ USER
Patient Comments	(0010,4000)	LT	Values supplied via Modality Worklist will be entered at <i>Patient Comment</i> . Comment from Modality Worklist or user input will be edited in the following format: <"Insurance="Health Insurance Information<LINEFEED> Comment>.	ALWAYS	MWL/ USER

**Table 8.1-6
GENERAL STUDY MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Study Instance UID	(0020,000D)	UI		ALWAYS	MWL/ AUTO
Study Date	(0008,0020)	DA		ALWAYS	AUTO
Study Time	(0008,0030)	TM		ALWAYS	AUTO
Referring Physician's Name	(0008,0090)	PN		VNAP	MWL/ USER
Study ID	(0020,0010)	SH		ALWAYS	AUTO
Accession Number	(0008,0050)	SH		VNAP	MWL/ USER
Study Description	(0008,1030)	LO	See Table 4.2-30 Notes	ALWAYS	MWL*/ USER
Study Comments	(0032,4000)	LT	Additional Info from user input will be edited in the following format: <"BSA="BSA Information<LINEFEED> "BSAType="BSA Type Information>.	ALWAYS	MWL/ USER
Referenced Study Sequence	(0008,1110)	SQ		ANAP	MWL
>Referenced SOP Class UID	(0008,1150)	UI		ANAP	MWL
>Referenced SOP Instance UID	(0008,1155)	UI		ANAP	MWL

**Table 8.1-7
PATIENT STUDY MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient's Age	(0010,1010)	AS		ANAP	AUTO
Patient's Size	(0010,1020)	DS		VNAP	MWL/ USER
Patient's Weight	(0010,1030)	DS		VNAP	MWL/ AUTO

**Table 8.1-8
GENERAL SERIES MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	US	ALWAYS	AUTO
Series Instance UID	(0020,000E)	UI		ALWAYS	AUTO
Series Number	(0020,0011)	IS		ALWAYS	AUTO
Series Date	(0008,0021)	DA		ALWAYS	AUTO
Series Time	(0008,0031)	TM		ALWAYS	AUTO
Performing Physician's Name	(0008,1050)	PN		VNAP	MWL/ USER
Protocol Name	(0018,1030)	LO		ALWAYS	AUTO
Series Description	(0018,103E)	LO	Blood Pressure from user input will be edited in the following format: <"BloodPressure="Blood Pressure Information>.	ANAP	AUTO
Operator's Name	(0008,1070)	PN		VNAP	USER
Referenced Performed Procedure Step Sequence	(0008,1111)	SQ		ANAP	MWL
>Referenced SOP Class UID	(0008,1150)	UI		ANAP	MWL
>Referenced SOP Instance UID	(0008,1155)	UI		ANAP	MWL
Request Attributes Sequence	(0040,0275)	SQ		ANAP	MWL
>Requested Procedure ID	(0040,1001)	SH		ANAP	MWL
>Scheduled Procedure Step ID	(0040,0009)	SH		ANAP	MWL
>Scheduled Procedure Step Description	(0040,0007)	LO	See Table 4.2-30 Notes	ANAP	MWL
>Scheduled Protocol Code Sequence	(0040,0008)	SQ		ANAP	MWL
Performed Procedure Step ID	(0040,0253)	SH		ANAP	AUTO
Performed Procedure Step Start Date	(0040,0244)	DA		ANAP	AUTO
Performed Procedure Step Start Time	(0040,0245)	TM		ANAP	AUTO
Performed Procedure Step Description	(0040,0254)	LO		ANAP	MWL
Performed Protocol Code Sequence	(0040,0260)	SQ		ANAP	MWL
>Code Value	(0008,0100)	SH		ANAP	AUTO
>Coding Scheme Designator	(0008,0102)	SH		ANAP	AUTO
>Coding Scheme Version	(0008,0103)	SH		ANAP	AUTO
>Code Meaning	(0008,0104)	LO		ANAP	AUTO

**Table 8.1-9
GENERAL EQUIPMENT MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Manufacturer	(0008,0070)	LO	TOSHIBA_MEC_US	ALWAYS	AUTO
Institution Name	(0008,0080)	LO		ALWAYS	CONFIG
Institution Address	(0008,0081)	ST		ALWAYS	CONFIG
Station Name	(0008,1010)	SH		ALWAYS	CONFIG
Institutional Department Name	(0008,1040)	LO		ALWAYS	CONFIG
Manufacturer's Model Name	(0008,1090)	LO	SSH-880CV	ALWAYS	AUTO
Device Serial Number	(0018,1000)	LO		ALWAYS	AUTO
Software Version	(0018,1020)	LO	AA_V1.50*R000	ALWAYS	AUTO

**Table 8.1-10
GENERAL IMAGE MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Instance Number	(0020,0013)	IS		ALWAYS	AUTO
Patient Orientation	(0020,0020)	CS		EMPTY	AUTO
Content Date	(0008,0023)	DA		ALWAYS	AUTO
Content Time	(0008,0033)	TM		ALWAYS	AUTO
Image Type	(0008,0008)	CS	Value 1: Pixel Data Characteristics "ORIGINAL" or "DERIVED" Value 2: Patient Exam Characteristics "PRIMARY" or "SECONDARY" Value 3: System Defined Term	ANAP	AUTO
Acquisition Date	(0008,0022)	DA		ALWAYS	AUTO
Acquisition Time	(0008,0032)	TM		ALWAYS	AUTO
Derivation Description	(0008,2111)	ST		ANAP	AUTO
Burned In Annotation	(0028,0301)	CS		ALWAYS	AUTO
Lossy Image Compression	(0028,2110)	CS		ANAP	AUTO
Lossy Image Compression Ratio	(0028,2112)	DS		ANAP	AUTO

**Table 8.1-11
IMAGE PIXEL MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Samples per Pixel	(0028,0002)	US		ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	CS		ALWAYS	CONFIG
Planar Configuration	(0028,0006)	US		ANAP	AUTO
Rows	(0028,0010)	US	720 or 1024	ALWAYS	AUTO
Columns	(0028,0011)	US	960 or 1280	ALWAYS	AUTO
Bits Allocated	(0028,0100)	US	8	ALWAYS	AUTO
Bits Stored	(0028,0101)	US	8	ALWAYS	AUTO
High Bit	(0028,0102)	US	7	ALWAYS	AUTO
Pixel Representation	(0028,0103)	US	0	ALWAYS	AUTO
Pixel Data	(7FE0,0010)	OB or OW		ALWAYS	AUTO

**Table 8.1-12
PRIVATE APPLICATION MODULE OF CREATED SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Private Creator	(0029,00xx)	LO		ALWAYS	AUTO
Application Header Type	(0029,xx08)	CS		ALWAYS	AUTO
Application Header Version	(0029,xx09)	LO		ALWAYS	AUTO
Application Header Data	(0029,xx10)	OB		ALWAYS	AUTO
Application Header Type	(0029,xx89)	LO		ALWAYS	AUTO
Application Header Data	(0029,xx90)	OB		ALWAYS	AUTO
Private Creator	(7015,00xx)	LO		ALWAYS	AUTO
Application Header Data	(7015,xx60)	OB		ANAP	AUTO
Application Header Sequence	(7015,xx73)	SQ		ALWAYS	AUTO

8.1.1.6 US Region Calibration Module

Table 8.1-13
US REGION CALIBRATION MODULE

Attribute Name	Tag	VR	Value	Presence of Value	Source
Sequence of Ultrasound Regions	(0018,6011)	SQ		ALWAYS	AUTO
>Region Spatial Format	(0018,6012)	US		ALWAYS	AUTO
>Region Data Type	(0018,6014)	US		ALWAYS	AUTO
>Region Flags	(0018,6016)	UL		ALWAYS	AUTO
>Region Location Min x0	(0018,6018)	UL		ALWAYS	AUTO
>Region Location Min y0	(0018,601A)	UL		ALWAYS	AUTO
>Region Location Max x1	(0018,601C)	UL		ALWAYS	AUTO
>Region Location Max y1	(0018,601E)	UL		ALWAYS	AUTO
>Reference Pixel x0	(0018,6020)	SL		ALWAYS	AUTO
>Reference Pixel y0	(0018,6022)	SL		ALWAYS	AUTO
>Physical Units X Direction	(0018,6024)	US		ALWAYS	AUTO
>Physical Units Y Direction	(0018,6026)	US		ALWAYS	AUTO
>Reference Pixel Physical Value X	(0018,6028)	FD		ALWAYS	AUTO
>Reference Pixel Physical Value Y	(0018,602A)	FD		ALWAYS	AUTO
>Physical Delta X	(0018,602C)	FD		ALWAYS	AUTO
>Physical Delta Y	(0018,602E)	FD		ALWAYS	AUTO
>Transducer Frequency	(0018,6030)	UL		ALWAYS	AUTO
>Pulse Repetition Frequency	(0018,6032)	UL		ANAP	AUTO
>Doppler Correction Angle	(0018,6034)	FD		ANAP	AUTO
>Steering Angle	(0018,6036)	FD		ANAP	AUTO
>Doppler Sample Volume X Position	(0018,6038)	UL		ANAP	AUTO
>Doppler Sample Volume Y Position	(0018,603A)	UL		ANAP	AUTO
>TM-Line Position x0	(0018,603C)	UL		ANAP	AUTO
>TM-Line Position y0	(0018,603E)	UL		ANAP	AUTO
>TM-Line Position x1	(0018,6040)	UL		ANAP	AUTO
>TM-Line Position y1	(0018,6042)	UL		ANAP	AUTO

8.1.1.7 SC Image Modules

Table 8.1-14
SC EQUIPMENT MODULE OF CREATED SC IMAGE SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Conversion Type	(0028,0064)	CS	“DV” (Digitized Video), “DI” (Digital Interface), “DF” (Digitized Film), or “WSD” (Workstation)	ALWAYS	AUTO

Table 8.1-15
SC IMAGE MODULE OF CREATED SC IMAGE SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Date of Secondary Capture	(0018,1012)	DA		Not Present	
Time of Secondary Capture	(0018,1014)	TM		Not Present	

Table 8.1-16
SOP COMMON MODULE OF CREATED SC IMAGE SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Specific Character Set	(0008,0008)	CS	ISO_IR 100	ALWAYS	AUTO
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.7	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI		ALWAYS	AUTO

8.1.1.8 US Image Modules

Table 8.1-17
US IMAGE MODULE OF CREATED US IMAGE SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Transducer Data	(0018,5010)	LO		ALWAYS	AUTO
Focus Depth	(0018,5012)	DS		ALWAYS	AUTO
Mechanical Index	(0018,5022)	DS		ALWAYS	AUTO
Bone Thermal Index	(0018,5024)	DS		ALWAYS	AUTO
Soft Tissue Thermal Index	(0018,5027)	DS		ALWAYS	AUTO
Depth of Scan Field	(0018,5050)	IS		ALWAYS	AUTO
Transducer Type	(0018,6031)	CS		ALWAYS	AUTO
Samples per Pixel	(0028,0002)	US		ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	CS		ALWAYS	CONFIG
Planar Configuration	(0028,0006)	US		ANAP	AUTO
Rows	(0028,0010)	US	720	ALWAYS	USER
Columns	(0028,0011)	US	960	ALWAYS	USER
Ultrasound Color Data Present	(0028,0014)	US		ALWAYS	AUTO
Bits Allocated	(0028,0100)	US	8	ALWAYS	AUTO
Bits Stored	(0028,0101)	US	8	ALWAYS	AUTO
High Bit	(0028,0102)	US	7	ALWAYS	AUTO
Pixel Representation	(0028,0103)	US	0	ALWAYS	AUTO
Pixel Data	(7FE0,0010)	OB or OW		ALWAYS	AUTO

Table 8.1-18
SOP COMMON MODULE OF CREATED US IMAGE SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Specific Character Set	(0008,0008)	CS	ISO_IR 100	ALWAYS	AUTO
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.6.1	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI		ALWAYS	AUTO

8.1.1.9 US Multi-frame Image Modules

**Table 8.1-19
CINE MODULE OF CREATED US MULTI-FRAME IMAGE SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Start Trim	(0008,2142)	IS		ANAP	AUTO
Stop Trim	(0008,2143)	IS		ANAP	AUTO
Recommended Display Frame Rate	(0008,2144)	IS		ANAP	USER
Cine Rate	(0018,0040)	IS		ANAP	USER
Effective Duration	(0018,0072)	DS		ANAP	AUTO
Frame Time	(0018,1063)	DS		ALWAYS	AUTO
Frame Delay	(0018,1066)	DS		ANAP	AUTO
Actual Frame Duration	(0018,1242)	IS		ANAP	AUTO

**Table 8.1-20
MULTI-FRAME MODULE OF CREATED US MULTI-FRAME IMAGE SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Number of Frames	(0028,0008)	IS		ALWAYS	USER
Frame Increment Pointer	(0028,0009)	AT		ALWAYS	AUTO

**Table 8.1-21
US IMAGE MODULE OF CREATED US MULTI-FRAME IMAGE SOP INSTANCES**

Attribute Name	Tag	VR	Value	Presence of Value	Source
Stage Name	(0008,2120)	SH		ANAP	AUTO
Stage Number	(0008,2122)	IS		ANAP	AUTO
Number of Stages	(0008,2124)	IS		ANAP	AUTO
View Name	(0008,2127)	SH		ANAP	AUTO
View Number	(0008,2128)	IS		ANAP	AUTO
Number of Views in Stage	(0008,212A)	IS		ANAP	AUTO
Heart Rate	(0008,1088)	IS		ANAP	AUTO
Transducer Data	(0018,5010)	LO		ALWAYS	AUTO
Focus Depth	(0018,5012)	DS		ALWAYS	AUTO
Mechanical Index	(0018,5022)	DS		ALWAYS	AUTO
Bone Thermal Index	(0018,5024)	DS		ALWAYS	AUTO
Soft Tissue Thermal Index	(0018,5027)	DS		ALWAYS	AUTO
Depth of Scan Field	(0018,5050)	IS		ALWAYS	AUTO
Transducer Type	(0018,6031)	CS		ALWAYS	AUTO
Samples per Pixel	(0028,0002)	US		ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	CS		ALWAYS	AUTO
Planar Configuration	(0028,0006)	US		ALWAYS	AUTO
Rows	(0028,0010)	US	660 or 720	ALWAYS	AUTO
Columns	(0028,0011)	US	416, 480 or 960	ALWAYS	AUTO

Ultrasound Color Data Present	(0028,0014)	US		ANAP	AUTO
Bits Allocated	(0028,0100)	US	8	ALWAYS	AUTO
Bits Stored	(0028,0101)	US	8	ALWAYS	AUTO
High Bit	(0028,0102)	US	7	ALWAYS	AUTO
Pixel Representation	(0028,0103)	US	0	ALWAYS	AUTO
Stage Code Sequence	(0040,000A)	SQ		ANAP	AUTO
>Code Value	(0008,0100)	SH		ANAP	AUTO
>Coding Scheme Designator	(0008,0102)	SH		ANAP	AUTO
>Coding Scheme Version	(0008,0103)	SH		ANAP	AUTO
>Code Meaning	(0008,0104)	LO		ANAP	AUTO
View Code Sequence	(0054,0220)	SQ		ANAP	AUTO
>Code Value	(0008,0100)	SH		ANAP	AUTO
>Coding Scheme Designator	(0008,0102)	SH		ANAP	AUTO
>Coding Scheme Version	(0008,0103)	SH		ANAP	AUTO
>Code Meaning	(0008,0104)	LO		ANAP	AUTO
Pixel Data	(7FE0,0010)	OB		ALWAYS	AUTO

Table 8.1-22
SOP COMMON MODULE OF CREATED US MULTI-FRAME IMAGE SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Specific Character Set	(0008,0008)	CS	ISO_IR 100	ALWAYS	AUTO
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.3.1	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI		ALWAYS	AUTO

8.1.1.10 Enhanced SR Modules

Table 8.1-23
SR DOCUMENT SERIES MODULE OF CREATED ENHANCED SR SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	SR	ALWAYS	AUTO
Referenced Study Component Sequence	(0008,1111)	SQ		VNAP	AUTO
Series Instance UID	(0020,000E)	UI		ALWAYS	AUTO
Series Number	(0020,0011)	IS		ALWAYS	AUTO

Table 8.1-24
SR DOCUMENT GENERAL MODULE OF CREATED ENHANCED SR SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Content Date	(0008,0023)	DA		ALWAYS	AUTO
Content Time	(0008,0033)	TM		ALWAYS	AUTO
Instance Number	(0020,0013)	IS		ALWAYS	AUTO
Referenced Request Sequence	(0040,A370)	SQ		VNAP	AUTO
>Accession Number	(0008,0050)	SH		VNAP	MWL/ USER
>Referenced Study Sequence	(0008,1110)	SQ		VNAP	MWL
>Study Instance UID	(0020,000D)	UI		VNAP	MWL/ AUTO
>Requested Procedure Description	(0032,1060)	LO	See Table 4.2-30 Notes	VNAP	MWL/ USER
>Requested Procedure Code Sequence	(0032,1064)	SQ		VNAP	MWL
>Requested Procedure ID	(0040,1001)	SH		VNAP	MWL/ USER
>Placer Order Number/Imaging Service Request	(0040,2016)	LO		VNAP	MWL
>Filler Order Number/Imaging Service Request	(0040,2017)	LO		VNAP	MWL
Performed Procedure Code Sequence	(0040,A372)	SQ		ALWAYS	AUTO
Current Requested Procedure Evidence Sequence	(0040,A375)	SQ		VNAP	AUTO
>Referenced Series Sequence	(0008,1115)	SQ		VNAP	AUTO
>>Referenced SOP Sequence	(0008,1199)	SQ		VNAP	AUTO
>>>Referenced SOP Class UID	(0008,1150)	UI		VNAP	AUTO
>>>Referenced SOP Instance UID	(0008,1155)	UI		VNAP	AUTO
>>Series Instance UID	(0020,000E)	UI		ALWAYS	AUTO
>Study Instance UID	(0020,000D)	UI		VNAP	MWL/ AUTO
Completion Flag	(0040,A491)	CS	COMPLETE	ALWAYS	AUTO
Verification Flag	(0040,A493)	CS	UNVERIFIED	ALWAYS	AUTO

Table 8.1-25
SR DOCUMENT CONTENT MODULE OF CREATED ENHANCED SR SOP INSTANCES FOR
ECHOCARDIOGRAPHY PROCEDURE REPORT TEMPLATE

Attribute Name	Tag	VR	Value	Presence of Value	Source
Value Type	(0040,A040)	CS	CONTAINER	ALWAYS	AUTO
Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>Code Value	(0008,0100)	SH	125200	ALWAYS	AUTO
>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>Code Meaning	(0008,0104)	LO	Adult Echocardiography Procedure Report	ALWAYS	AUTO
Continuity of Content	(0040,A050)	CS	SEPARATE	ALWAYS	AUTO
Content Template Sequence	(0040,A504)	SQ		ALWAYS	AUTO
Template Identifier	(0040,DB00)	CS	5200	ALWAYS	AUTO
Mapping Resource	(0008,0105)	CS	DCMR	ALWAYS	AUTO
Content sequence	(0040,A730)	SQ		ALWAYS	AUTO
>Relationship Type	(0040,A010)	CS	HAS CONCEPT MOD	ALWAYS	AUTO
>Value Type	(0040,A040)	CS	CODE	ALWAYS	AUTO
>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>Code Value	(0008,0100)	SH	121049	ALWAYS	AUTO
>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>Code Meaning	(0008,0104)	LO	Language of Content Item and descendants	ALWAYS	AUTO
>Concept Code Sequence	(0040,A160)	SQ		ALWAYS	AUTO
>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>Relationship Type	(0040,A010)	CS	HAS OBS CONTEXT	ALWAYS	AUTO
>Value Type	(0040,A040)	CS	CODE	ALWAYS	AUTO
>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>Code Value	(0008,0100)	SH	121007	ALWAYS	AUTO
>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>Concept Code Sequence	(0040,A160)	SQ		ALWAYS	AUTO
>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>Value Type	(0040,A040)	CS	CONTAINER	ALWAYS	AUTO
>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>Code Value	(0008,0100)	SH	121118	ALWAYS	AUTO
>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>Code Meaning	(0008,0104)	LO	Patient Characteristics	ALWAYS	AUTO
>Content sequence	(0040,A730)	SQ		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	NUM	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	121033	ALWAYS	AUTO

>>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Subject Age	ALWAYS	AUTO
>>Measured Value Sequence	(0040,A300)	SQ		ALWAYS	AUTO
>>>Numeric Value	(0040,A30A)	DA		ALWAYS	AUTO
>>>Measured Units Code Sequence	(0040,08EA)	SQ		ALWAYS	AUTO
>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	CODE	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	121032	ALWAYS	AUTO
>>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Subject Sex	ALWAYS	AUTO
>>Concept Code Sequence	(0040,A160)	SQ		ALWAYS	AUTO
>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	NUM	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	8867-4	ALWAYS	AUTO
>>>Coding Scheme Designator	(0008,0102)	SH	LN	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Heart Rate	ALWAYS	AUTO
>>Measured Value Sequence	(0040,A300)	SQ		ALWAYS	AUTO
>>>Numeric Value	(0040,A30A)	DA		ALWAYS	AUTO
>>>Measured Units Code Sequence	(0040,08EA)	SQ		ALWAYS	AUTO
>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	NUM	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	F-008EC	ALWAYS	AUTO
>>>Coding Scheme Designator	(0008,0102)	SH	SRT	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Systolic Blood Pressure	ALWAYS	AUTO
>>Measured Value Sequence	(0040,A300)	SQ		ALWAYS	AUTO
>>>Numeric Value	(0040,A30A)	DA		ALWAYS	AUTO
>>>Measured Units Code Sequence	(0040,08EA)	SQ		ALWAYS	AUTO
>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	NUM	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	F-008ED	ALWAYS	AUTO

>>>Coding Scheme Designator	(0008,0102)	SH	SRT	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Diastolic Blood Pressure	ALWAYS	AUTO
>>Measured Value Sequence	(0040,A300)	SQ		ALWAYS	AUTO
>>>Numeric Value	(0040,A30A)	DA		ALWAYS	AUTO
>>>Measured Units Code Sequence	(0040,08EA)	SQ		ALWAYS	AUTO
>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	NUM	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	8277-6	ALWAYS	AUTO
>>>Coding Scheme Designator	(0008,0102)	SH	SRT	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Body Surface Area	ALWAYS	AUTO
>>Measured Value Sequence	(0040,A300)	SQ		ALWAYS	AUTO
>>>Numeric Value	(0040,A30A)	DA		ALWAYS	AUTO
>>>Measured Units Code Sequence	(0040,08EA)	SQ		ALWAYS	AUTO
>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>Value Type	(0040,A040)	CS	CONTAINER	ALWAYS	AUTO
>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>Code Value	(0008,0100)	SH	111028	ALWAYS	AUTO
>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>Code Meaning	(0008,0104)	LO	Image Library	ALWAYS	AUTO
>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>Value Type	(0040,A040)	CS	IMAGE	ALWAYS	AUTO
Referenced SOP Sequence	(0008,1199)	SQ		ALWAYS	AUTO
>Referenced SOP Class UID	(0008,1150)	UI		ALWAYS	AUTO
>Referenced SOP Instance UID	(0008,1155)	UI		ALWAYS	AUTO
>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>Value Type	(0040,A040)	CS	CONATINER	ALWAYS	AUTO
>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>Code Value	(0008,0100)	SH	121070	ALWAYS	AUTO
>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>Code Meaning	(0008,0104)	LO	Findings	ALWAYS	AUTO
>Content sequence	(0040,A730)	SQ		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	HAS CONCEPT MOD	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	CODE	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	G-C0E3	ALWAYS	AUTO
>>>Coding Scheme Designator	(0008,0102)	SH	SRT	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Finding Site	ALWAYS	AUTO
>>Concept Code Sequence	(0040,A160)	SQ		ALWAYS	AUTO
>>>Code value	(0008,0100)	SH		ALWAYS	AUTO

>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>Value Type	(0040,A040)	CS	CONTAINER	ALWAYS	AUTO
>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>Code Value	(0008,0100)	SH	125007	ALWAYS	AUTO
>>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>>Code Meaning	(0008,0104)	LO	Measurement Group	ALWAYS	AUTO
>>Content sequence	(0040,A730)	SQ		ALWAYS	AUTO
>>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>>Value Type	(0040,A040)	CS	CODE	ALWAYS	AUTO
>>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>>Code Value	(0008,0100)	SH	R-4089A	ALWAYS	AUTO
>>>>Coding Scheme Designator	(0008,0102)	SH	SRT	ALWAYS	AUTO
>>>>Code Meaning	(0008,0104)	LO	Cardiac Cycle Point	ALWAYS	AUTO
>>>Concept Code Sequence	(0040,A160)	SQ		ALWAYS	AUTO
>>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>>Value Type	(0040,A040)	CS	CODE	ALWAYS	AUTO
>>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>>Code Value	(0008,0100)	SH	111031	ALWAYS	AUTO
>>>>Coding Scheme Designator	(0008,0102)	SH	DCM	ALWAYS	AUTO
>>>>Code Meaning	(0008,0104)	LO	Image view	ALWAYS	AUTO
>>>Concept Code Sequence	(0040,A160)	SQ		ALWAYS	AUTO
>>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>>Relationship Type	(0040,A010)	CS	CONTAINS	ALWAYS	AUTO
>>>Value Type	(0040,A040)	CS	NUM	ALWAYS	AUTO
>>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>>Code Value	(0008,0100)	SH		ALWAYS	AUTO
>>>>Coding Scheme Designator	(0008,0102)	SH		ALWAYS	AUTO
>>>>Code Meaning	(0008,0104)	LO	Measurement name or description	ALWAYS	AUTO
>>>Measured Value Sequence	(0040,A300)	SQ		ALWAYS	AUTO
>>>>Numeric Value	(0040,A30A)	DA		ALWAYS	AUTO
>>>Measured Units Code Sequence	(0040,08EA)	SQ		ALWAYS	AUTO
>>>>Code value	(0008,0100)	SH		ALWAYS	AUTO
>>>>Coding Scheme designator	(0008,0102)	SH		ALWAYS	AUTO
>>>>Code Meaning	(0008,0104)	LO		ALWAYS	AUTO
>>>Relationship Type	(0040,A010)	CS	HAS CONCEPT MOD	ALWAYS	AUTO
>>>Value Type	(0040,A040)	CS	CODE	ALWAYS	AUTO
>>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>>Code Value	(0008,0100)	SH	G-C036	ALWAYS	AUTO
>>>>Coding Scheme Designator	(0008,0102)	SH	SRT	ALWAYS	AUTO

>>>>Code Meaning	(0008,0104)	LO	Measurement Method	ALWAYS	AUTO
>>>Concept Name Code Sequence	(0040,A043)	SQ		ALWAYS	AUTO
>>>>Code Value	(0008,0100)	SH		ALWAYS	AUTO
>>>>Coding Scheme Designator	(0008,0102)	SH		ALWAYS	AUTO
>>>>Code Meaning	(0008,0104)	LO	Method	ALWAYS	AUTO

Table 8.1-26
SOP COMMON MODULE OF CREATED ENHANCED SR SOP INSTANCES

Attribute Name	Tag	VR	Value	Presence of Value	Source
Specific Character Set	(0008,0008)	CS	ISO_IR 100	ALWAYS	AUTO
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.88.22	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI		ALWAYS	AUTO

8.1.2 Usage of Attributes from received IOD's

No SOP Class specific fields are required.

8.1.3 Attribute Mapping

The relationships between attributes received via Modality Worklist, stored in acquired images and communicated via MPPS are summarized in Table 8.1-27.

**Table 8.1-27
ATTRIBUTE MAPPING BETWEEN MODALITY WORKLIST, IMAGE AND MPPS**

Modality Worklist	Image IOD	MPPS IOD
--	--	Scheduled Step Attribute Sequence
Study Instance UID	Study Instance UID	>Study Instance UID
Referenced Study Sequence	Referenced Study Sequence	>Referenced Study Sequence
Accession Number	Accession Number	>Accession Number
--	Request Attributes Sequence	--
Requested Procedure ID	>Requested Procedure ID	>Requested Procedure ID
Scheduled Procedure Step ID	>Scheduled Procedure Step ID	>Scheduled Procedure Step ID
Scheduled Procedure Step Description	>Scheduled Procedure Step Description	>Scheduled Procedure Step Description
Scheduled Protocol Code Sequence	>Scheduled Protocol Code Sequence	--
Requested Procedure ID	Study ID	Study ID
--	Performed Procedure Step ID	Performed Procedure Step ID
--	Performed Procedure Step Description	Performed Procedure Step Description
Requested Procedure Description		
Requested Procedure Code Sequence	Procedure Code Sequence	Procedure Code Sequence

8.1.4 Coerced/Modified Fields

Not applicable.

8.2 DATA DICTIONARY OF PRIVATE ATTRIBUTES

This product reserves private attribute values in the groups 0029 and 7015.
The private attributes added to created SOP instances or directory records are listed in Table 8.1-12.

8.3 CONTROLLED TERMINOLOGY AND TEMPLATES

Not applicable.

8.4 GRAYSCALE IMAGE CONSISTENCY

Not applicable.

8.5 STANDARD EXTENDED/SPECIALIZED/PRIVATE SOP CLASSES

Not applicable.

8.6 PRIVATE TRANSFER SYNTAXES

Not applicable.